


File D:\DATA\A02\RS-J147-01005-HPLCA004.D
 Injection Date : 11-Dec-15, 08:38:49 Tgt Mass (EZX) :
 Sample Name : J147 01 Location : P1-B-03
 Acq. Operator : HPLCA004 Inj : 0
 Spec. Reported : MS Integration Inj Volume : 3 ul
 Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
 Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
 Sample Info : Easy-Access Method: '2-HPLC-15min'
 Method Info : Mobile Phase: A: water (0.01%TFA) B: ACN (0.01%TFA)
 Gradient: 0min 5%B, 3min 5%B, 10min 95%B, 15min 95%B
 Flow Rate: 1.2 ml/min
 Column: Eclipse XDB-C18, 4.6*150mm, 5um
 Oven Temperature: 40 C

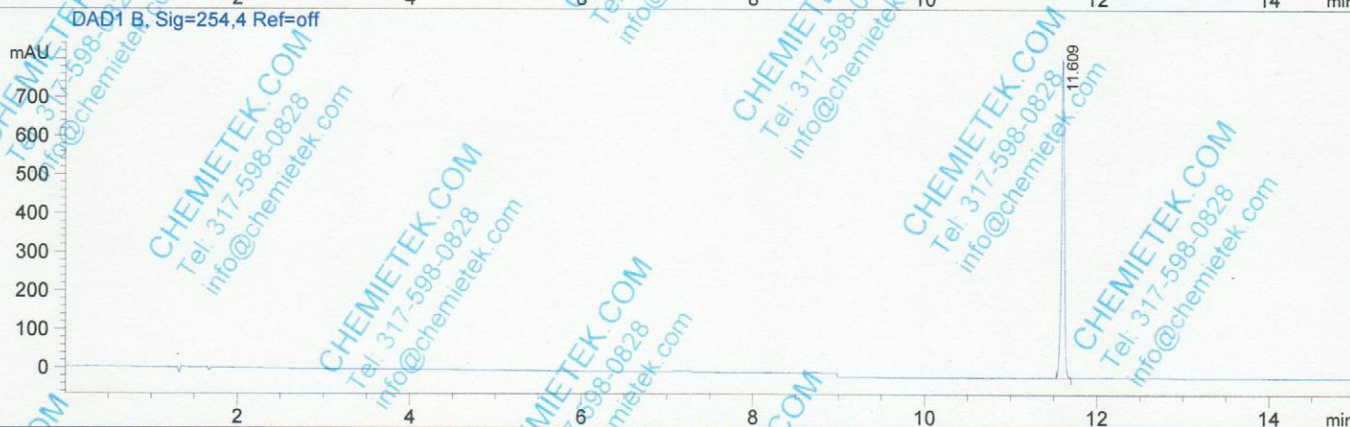

Integration Results for DAD1 A, Sig=214.4 Ref=off

RetTim	Width	Area	Height	Area%
11.61	0.04	4816.51	1778.12	100.00

Integration Results for DAD1 B, Sig=254.4 Ref=off

RetTim	Width	Area	Height	Area%
11.61	0.04	2008.40	823.92	100.00

