




Chiral HPLC Report


Sample Information

Sample ID: Default
Compound ID: CFT-1946 Lot 01
Acq Method: Default

Channel Name: 220
Project Name: CTK\SFC-H-Default
User Name: Default_CA
Instrument: Waters UPCC with SQ Detector 2

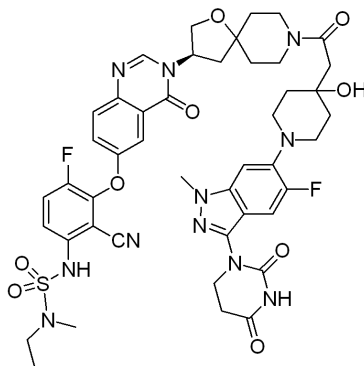

Test Results

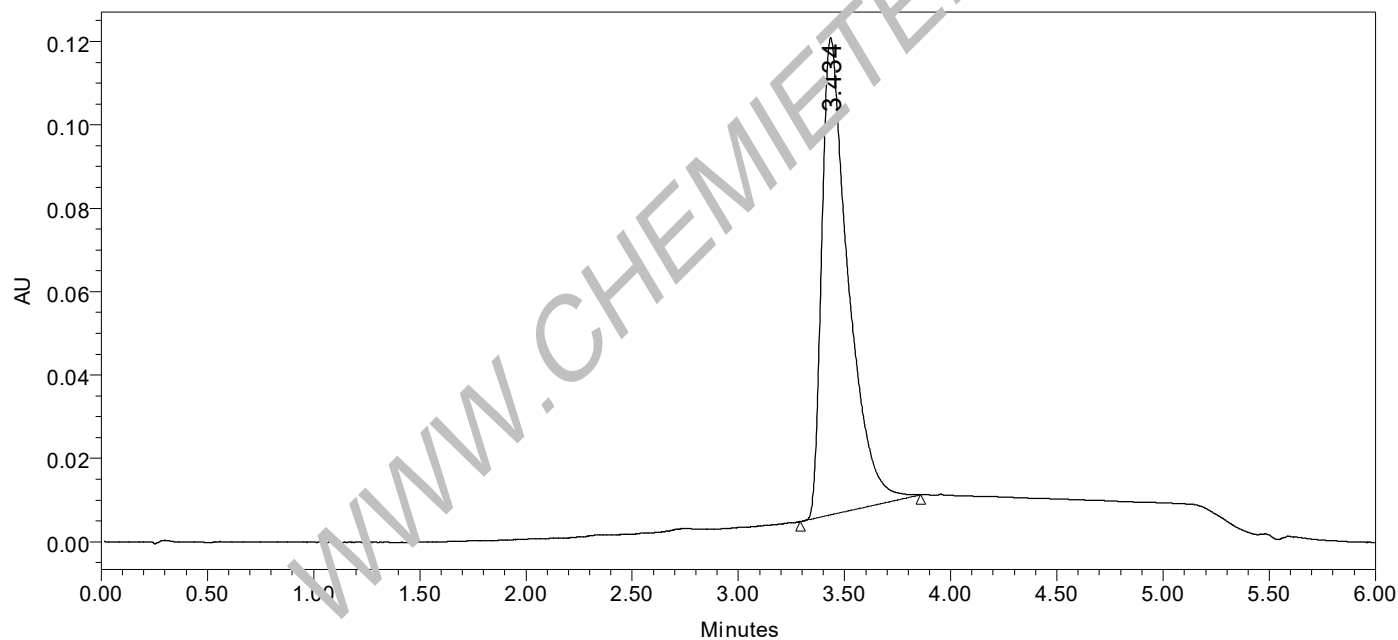

	RT	Area	% Area	Height
1	3.434	992169	100.00	114463