HPLC REPORT

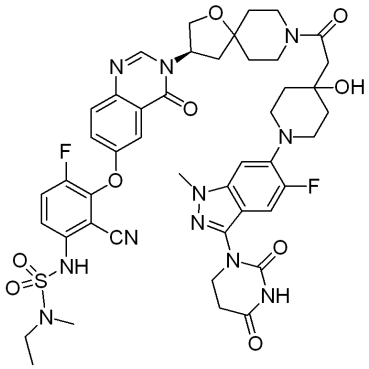

Compound ID : CFT-1946, Lot 01
Sample ID : Default
Injection Vol : 2ul
Acq Method : D: Method\HPLC-079_CHEMIELAB_20min.lcm
Instrument : HPLC-079

==========

Method Information

Instrument:Shimadzu LC-20AD
Mobile Phase:A:0.04%TFA in H2O
Mobile Phase:B:0.02%TFA in ACN
Flow :1.2000
Column Temperature:40 C

WWW.CHEMIETEK.COM

Chromatogram

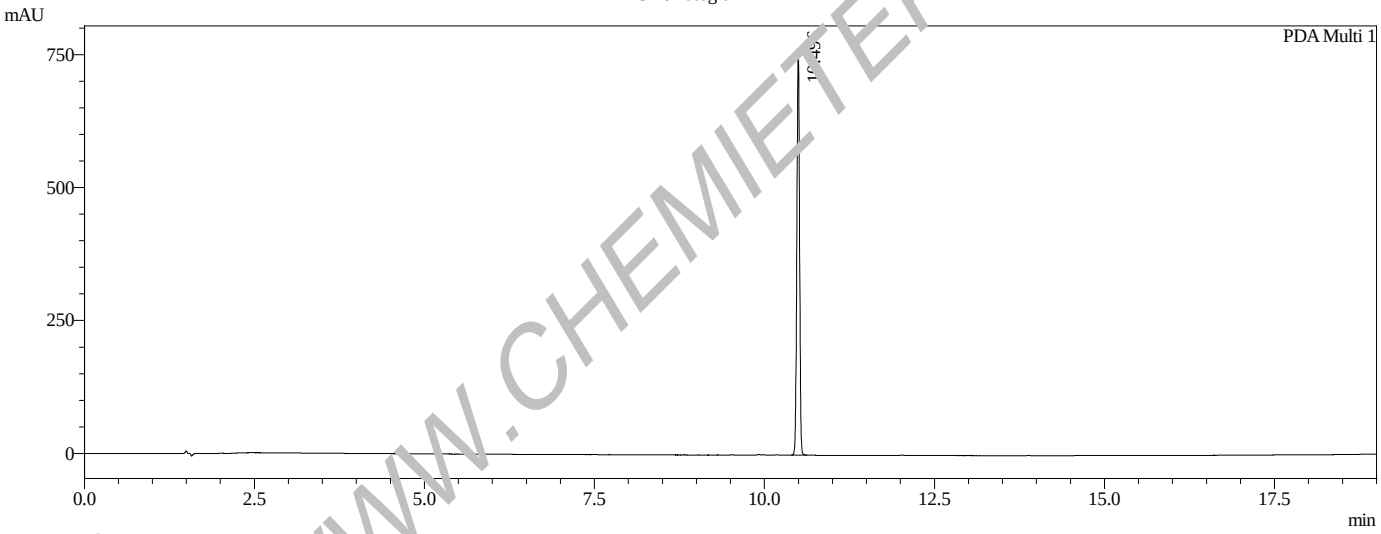

1 PDA Multi 1 / 220nm 4nm

==========

Integration Result

==========

PDA Ch1 220nm 4nm

Peak#	Ret. Time	Height	Height %	USP Width	Area	Area %
1	10.496	764166	100.000	0.076	2099482	100.000