



# CHEMIETEK Chiral HPLC Report

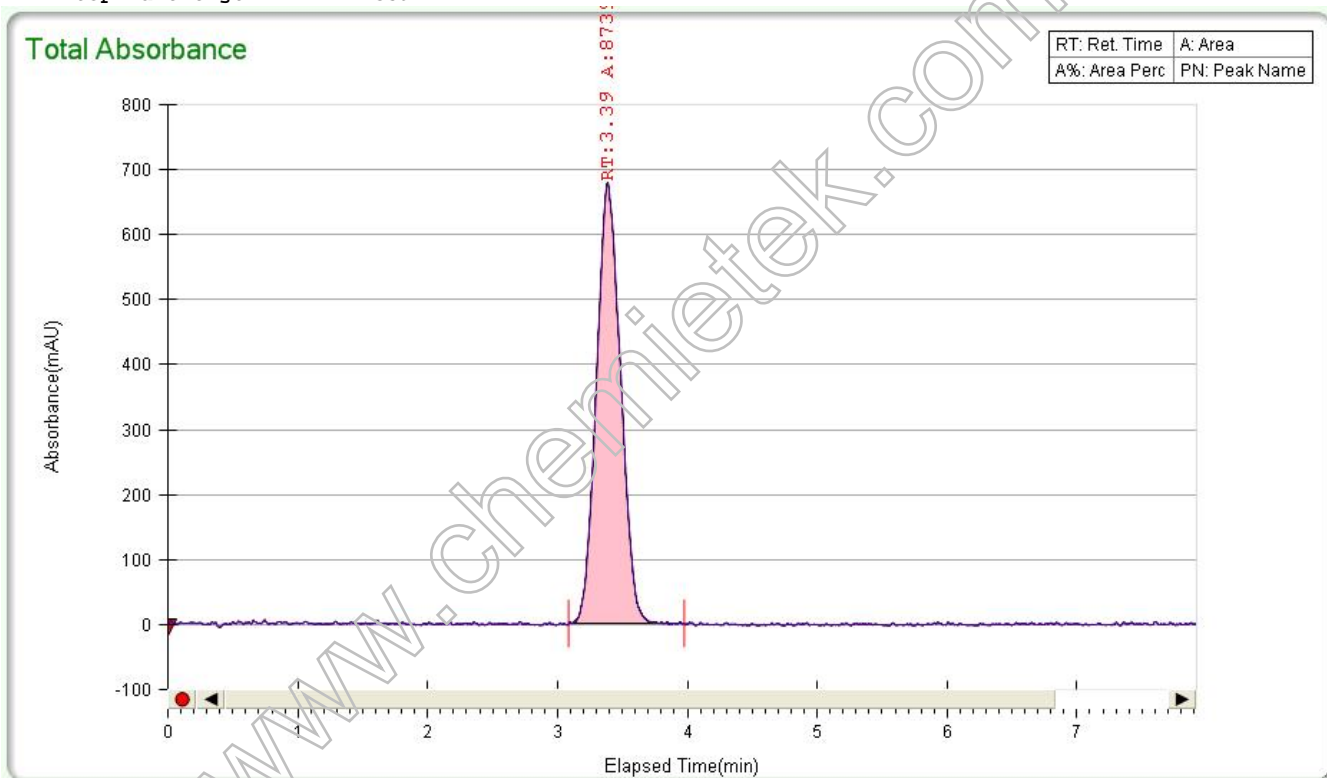

## Injection Info

Injection Volume 3  
Co-Solvent  
Column  
Sample GS-9901-Chemietek-01  
Sample Well P1: 1E  
Column Temperature 40.3  
CO2 Flow Rate 2.8  
Co-Solvent Flow Rate 1.2  
Co-Solvent % 30  
Total Flow 4  
Front Pressure 153  
Back Pressure 124  
Pressure Drop 29  
PDA Start Wavelength 214  
PDA Stop Wavelength 359

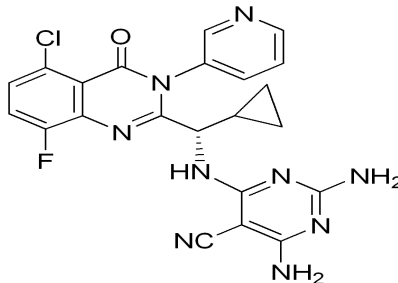

## Peak Info

Number	RT (min)	Area %	Area	Height
1	3.39	100	8739.3086	678.4899