





Chiral HPLC Analysis Report

Injection Volume 1
Co-Solvent MeOH(0.2%Methanol Ammonia)
Column OD-H (4.6*100mm, 5um)
Sample PD-0325901 04
Sample Well P1: 4A
Column Temperature 37.6
CO2 Flow Rate 3.4
Co-Solvent Flow Rate 0.6
Co-Solvent % 15
Back Pressure 119
Total Flow 4
PDA Start Wavelength 214
PDA Stop Wavelength 359
Injection Info

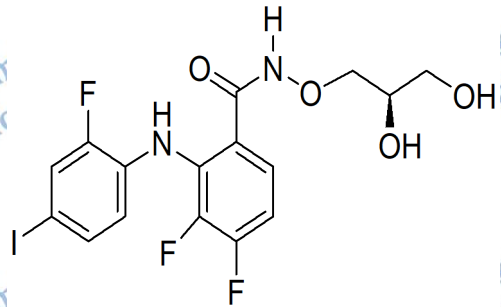

Number	RT (min)	Area	Area %	Theoretical Plate
1	2.49	4371.682	100	1976.2405

Peak Info

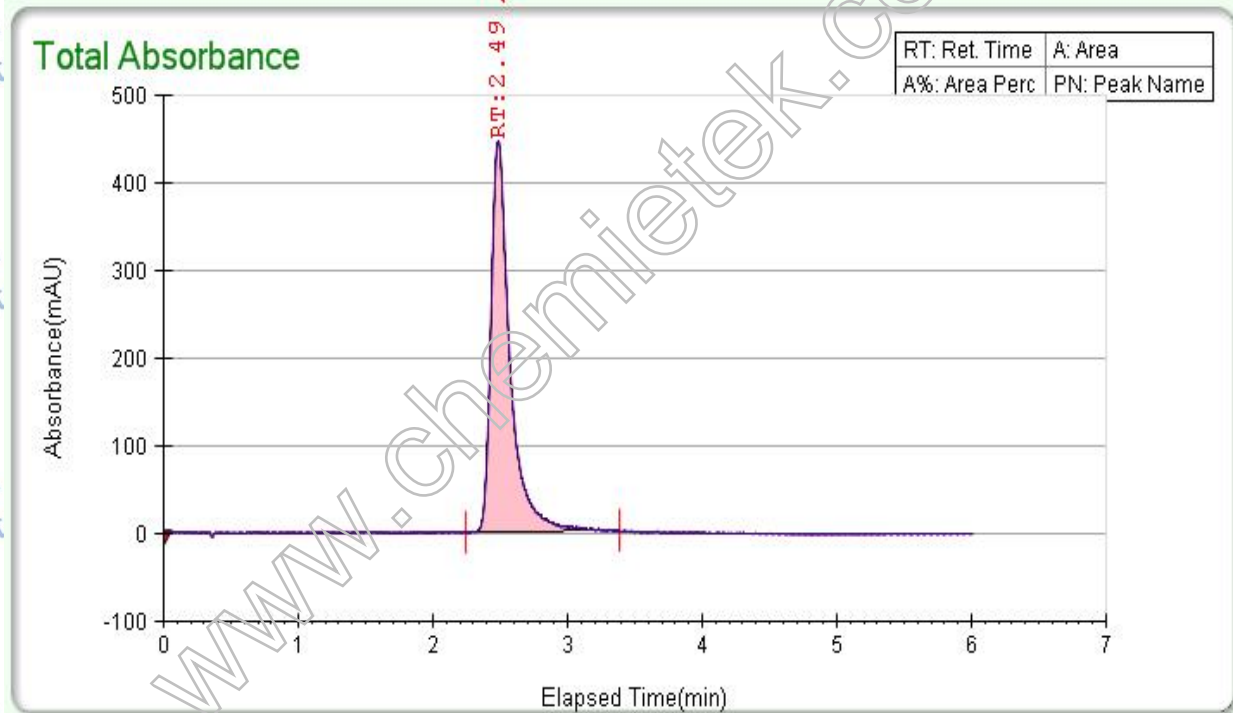

PDASingleSpectrumGraph
PDASingleSpectrumPlot.png