

CHEMIETEK HPLC-MS Report




File D:\DATA\A02\MONITOR\RS-CR-2-02864-LCMSA015.D

Sample Name : PF-02341066,-R-Crizo, 08  
 Acq. Operator : LCMSA015  
 Spec. Reported : MS Integration  
 Acq. Method : C:\Chem32\1\METHODS\1-POS-3MIN.M  
 Analysis Method : C:\Chem32\1\METHODS\1-POS-3MIN.M  
 Sample Info : \*\*\* No target masses specified \*\*\*

Tgt Mass(EZX) :  
 Location : P1-C-01  
 Inj : 1  
 Inj Volume : 1 ul



Method Info : Mobile Phase : A:H2O (0.01%TFA) B:MeCN (0.01%TFA)  
 Gradient: 5%-95% B in 1.2min  
 Flow Rate : 2 ml/min  
 Column : SunFire C18 50\*4.6mm,3.5um  
 Oven Temperature: 45 C  
 mass range :50-800

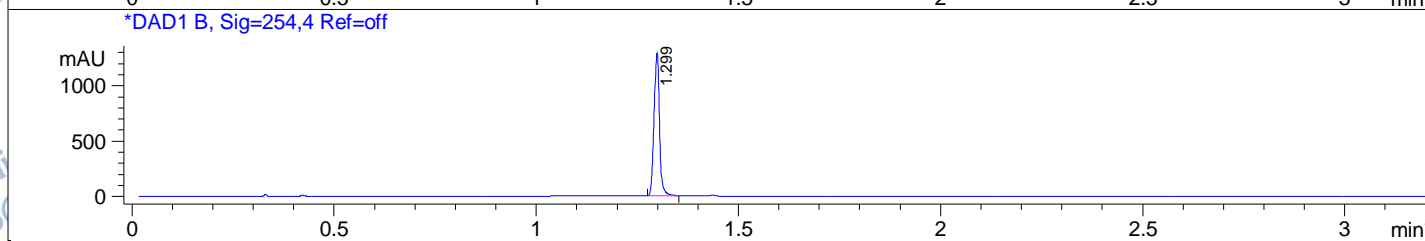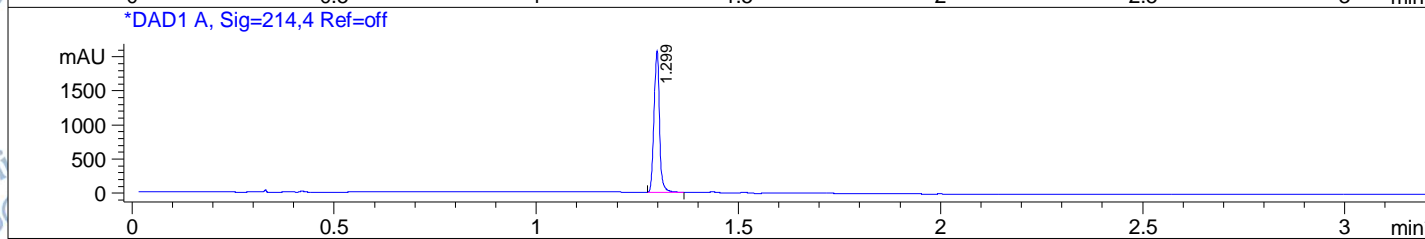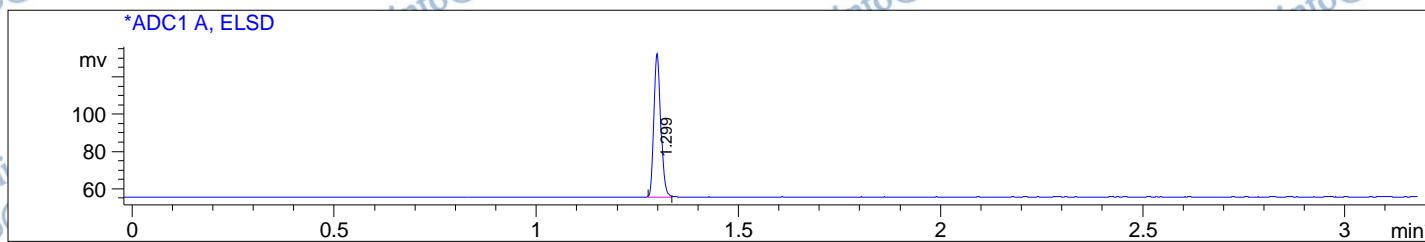

Integration Results for ADC1 A, ELSD


RetTim	Width	Area	Height	Area%
1.30	0.02	93.35	76.93	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.30	0.01	1973.62	2081.03	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.30	0.01	1226.72	1294.90	100.00

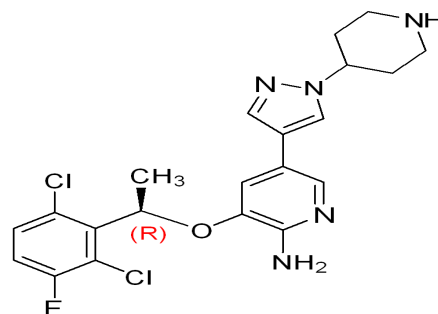

Ret. Time: 1.30

<<<< POSITIVE SPECTRA >>>>

