
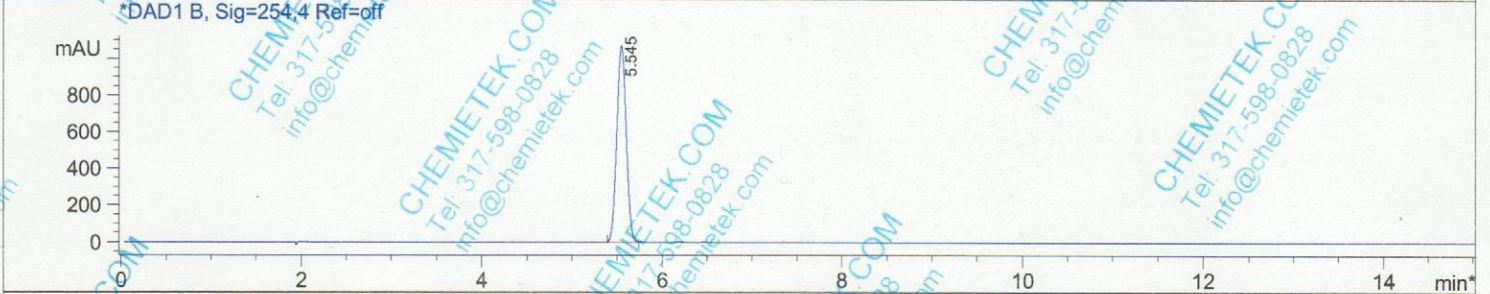
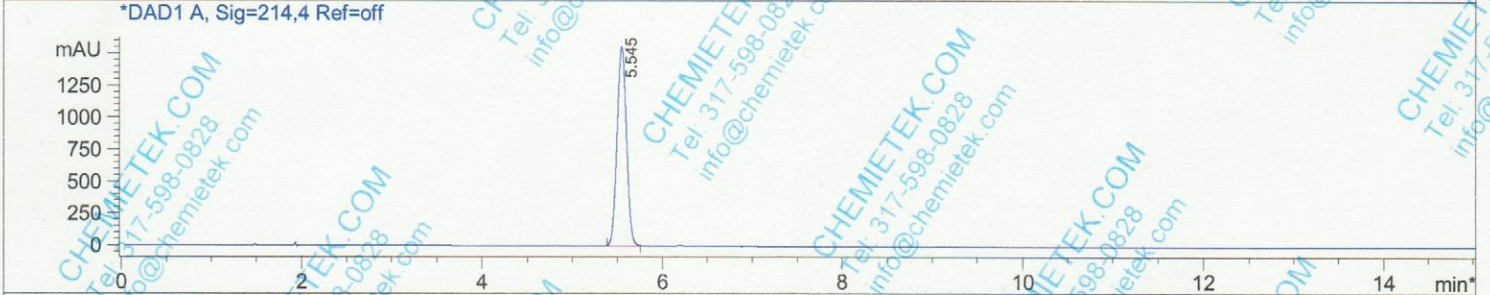


File ..TA\A02\MONITOR\ACP196-02-2-00586-LCMSA033.D Tgt Mass (EZX):  
 Injection Date : 22 Jul 16 5:09 pm +0800 Seq. Line : 0  
 Sample Name : ACP196-02 Location : P1-E-01  
 Acq. Operator : A02-MONITOR Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 3 ul  
 Acq. Method : D:\METHODS\2-HPLC-HIYN.M  
 Analysis Method : D:\METHODS\2-HPLC-HIYN.M  
 Sample Info : Easy-Access Method: '2-HPLC-HIYN'  
 Method Info : Mobile Phase: A: water (10mMNH4HCO3) B: ACN  
 Gradient  
 Time 0 7.5 15  
 B % 5 95 95  
 Flow Rate: 1.0mL/min  
 Oven temperature: 50C

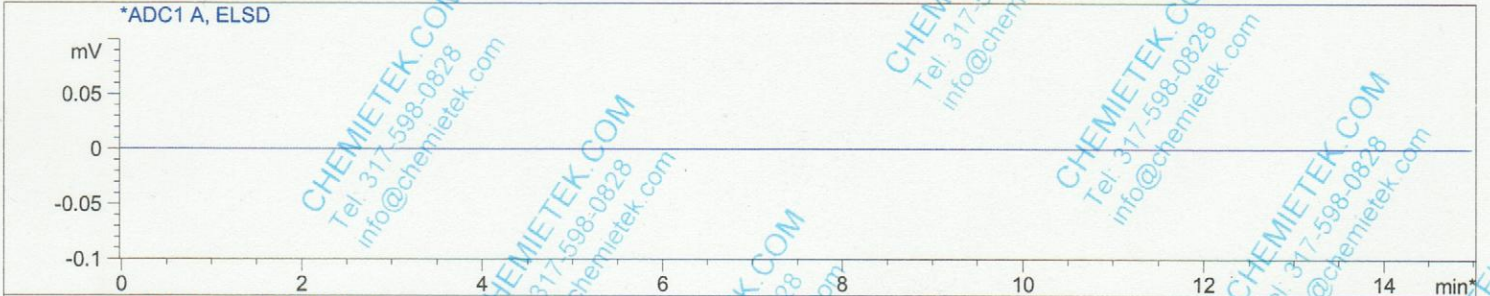

Integration Results for ADC1 A, ELSD


RetTim	Width	Area	Height	Area%
--------	-------	------	--------	-------

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.55	0.11	11388.87	1555.09	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.55	0.11	7815.75	1069.46	100.00

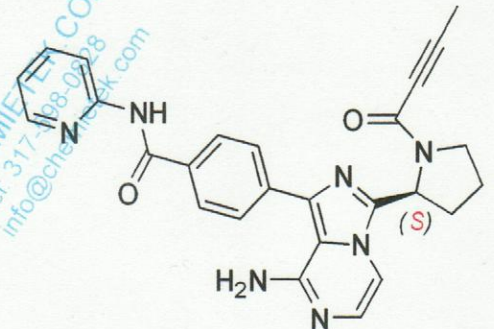

Ret. Time: 5.54

