

File D:\DATA\A02\MONITOR\AG-221-01-34810-LCMSA002.D

Injection Date : 3 May 16 12:53 pm +0800

Tgt Mass (EZX) :

Sample Name : AG-221-01

Location : P2-C-01

Acq. Operator : A02-MONITOR

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : D:\METHODS\1-POS-3MIN-MON.M

Analysis Method : D:\METHODS\1-POS-3MIN-MON.M

Sample Info : Easy-Access Method: '1-POS-3MIN-MON'




Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)

Gradient: 5% to 95%B within 1.6 min

Flow Rate :2.0ml/min

Column :SunFire C18, 4.6*50mm,3.5um

Oven Temperature : 50C

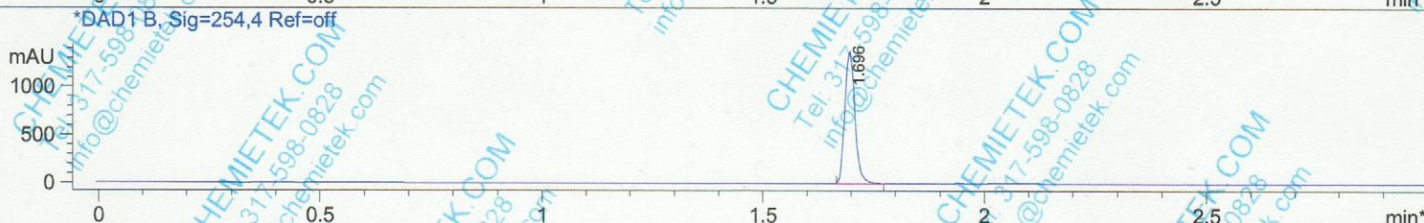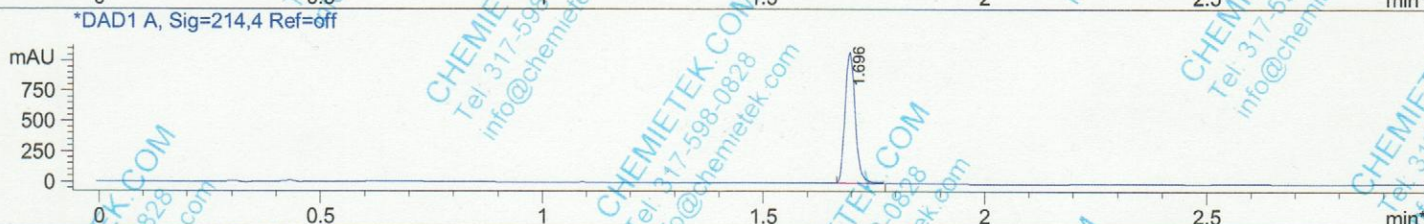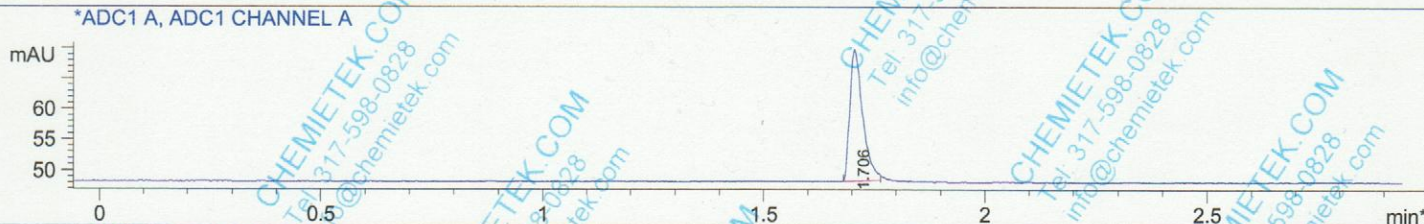

Integration Results for ADC1 A, ADC1 CHANNEL A


RetTim	Width	Area	Height	Area%
1.71	0.03	43.14	21.55	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.70	0.02	1734.76	1088.88	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.70	0.02	2181.51	1380.83	100.00

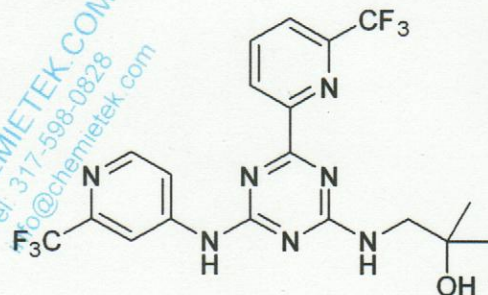

CHEMIETEK HPLC/MS Report

Ret. Time: 1.70

