




## SAMPLE INFORMATION

Sample ID:	Default	Acquired By:	System
Compound ID:	ARS-1620_01	Sample Set Name:	0507_10_1
Acq Method :		Processing Method:	1
Date Acquired:	2019/5/7 19:13:40 CST	Injection Volume:	1.00 ul
Date Processed:	2019/5/8 10:06:45 CST	Vial:	2:B,5
Proc. Chnl. Descr.:	PDA Ch1 220nm@4.8nm	Run Time:	6.0 Minutes
Channel Name:	PDA Ch1 220nm@4.8nm		
Instrument:	CAS-CTK-ANA-SFC-3(Waters UPCC with PDA detector)		

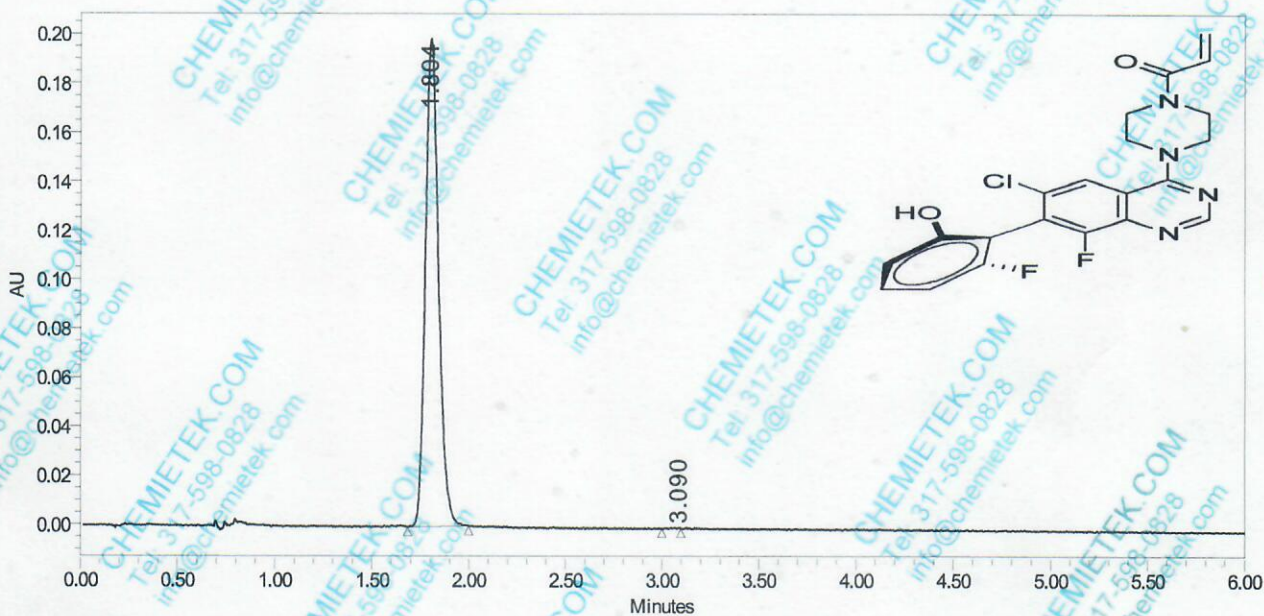

	RT	Area	% Area	Height
1	1.804	935887	99.85	199164
2	3.090	1438	0.15	409