CHEMIETEK HPLC Report

File D:\DATABACKUP\RAWDATA\C52\LCMS\MONITOR\2019-06\2019-06-22\
Injection Date : 22 Jun 19 3:06 pm +0800 Tgt Mass(EZX) : 460.00
Sample Name : CT-ASN002 Lot 01 Location : P1-A-01
Acq. Operator : C52-MONITOR Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\METHODS\2-HPLC-15MIN.M
Analysis Method : D:\METHODS\2-HPLC-15MIN.M
Sample Info : Easy-Access Method: '2-HPLC.M' 460.00 Method
Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.
Flow Rate: 1.0ml/min
Column:Sunfire C18,4.6*150mm,3.5um
Column Temperature: 45 C
Detection:UV(254,4nm) and MS(ESI,Pos mode,110 to 1500 amu)

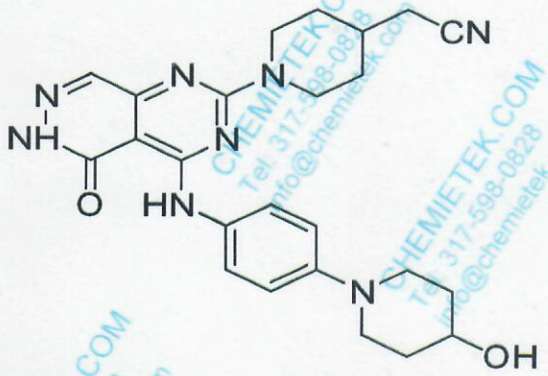


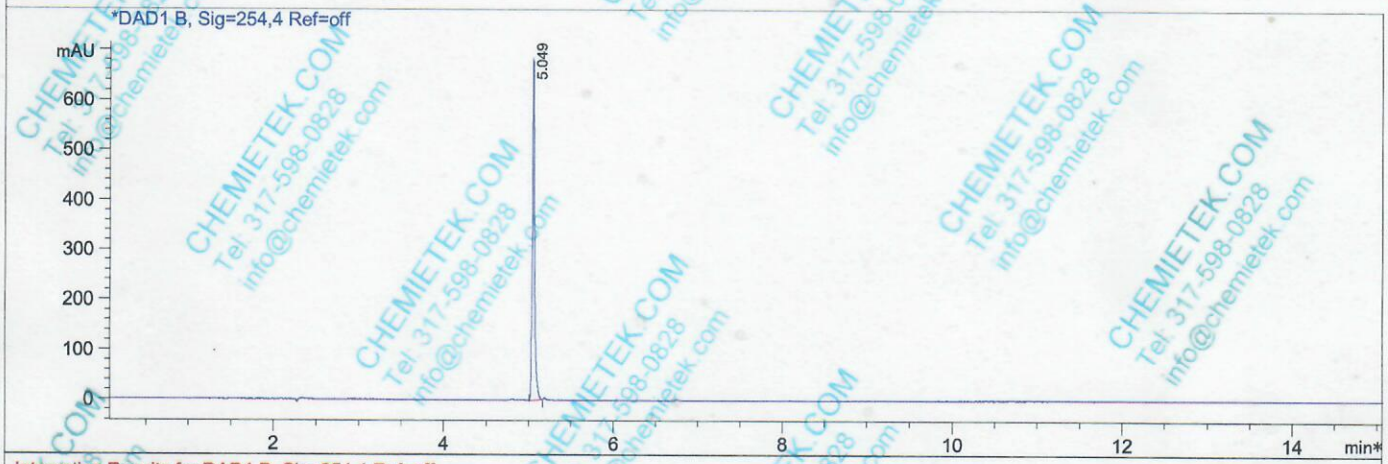


Integration Results for DAD1 B, Sig=254,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|---|---|---|---|---|
| 5.05 | 0.03 | 1350.01 | 684.16 | 100.00 |

CHEMIETEK.COM Tel: 317-598-0828 info@chemietek.com