HPLC Report

File D:\DATA\C52\MONITOR\CTK-0022259-006-06425-LCMSA013.D
Injection Date : 23-Jul-19, 18:07:17 Tgt Mass(EZX) :
Sample Name : CT-AZD3458 01 Location : P1-D-07
Acq. Operator : C52-MONITOR Inj : 0
Spec. Reported : MS Integration Inj Volume : 3 ul
Acq. Method : D:\METHODS\2-HPLC-15MIN.M
Analysis Method : D:\METHODS\2-HPLC-15MIN.M
Sample Info : Easy-Access Method: '2-HPLC.M'
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.
Flow Rate: 1.0ml/min
Column:Sunfire C18,4.6*150mm,3.5um
Column Temperature: 45 C

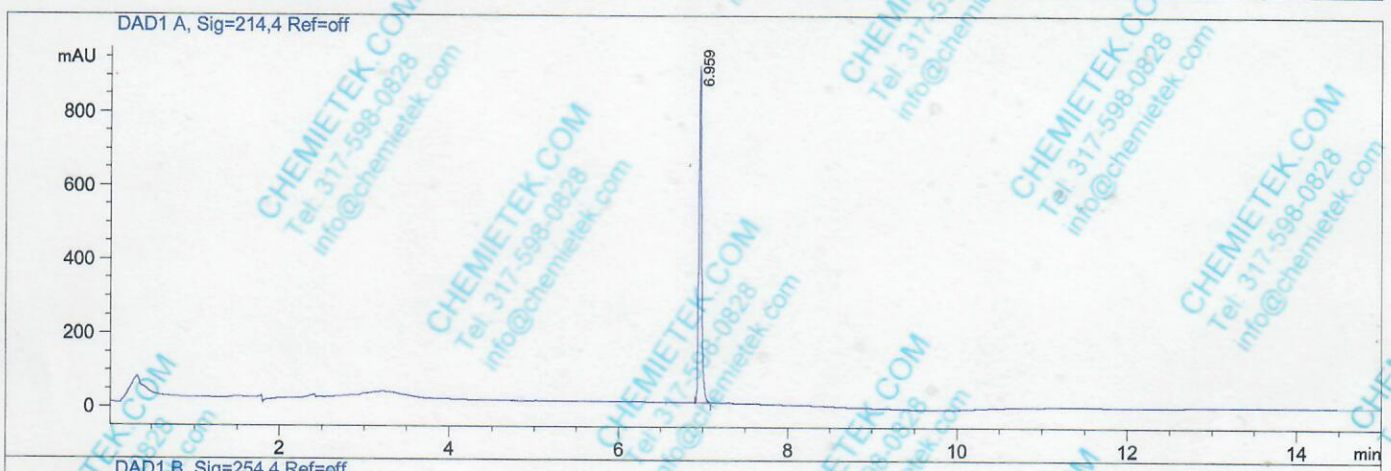

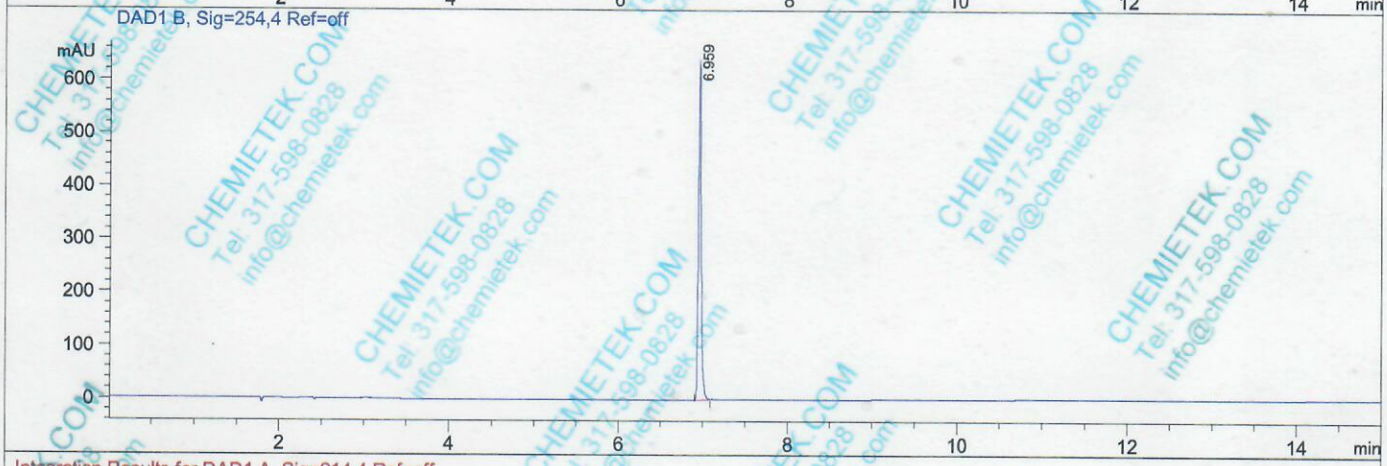

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
6.96	0.03	2086.52	915.56	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.96	0.03	1446.85	639.68	100.00

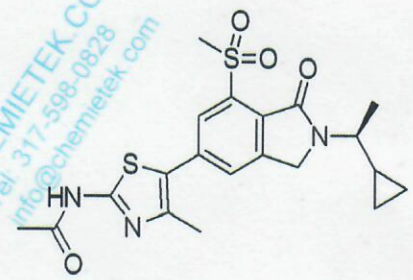

CHEMIETEK.COM Tel: 317-598-0828 info@chemietek.com