
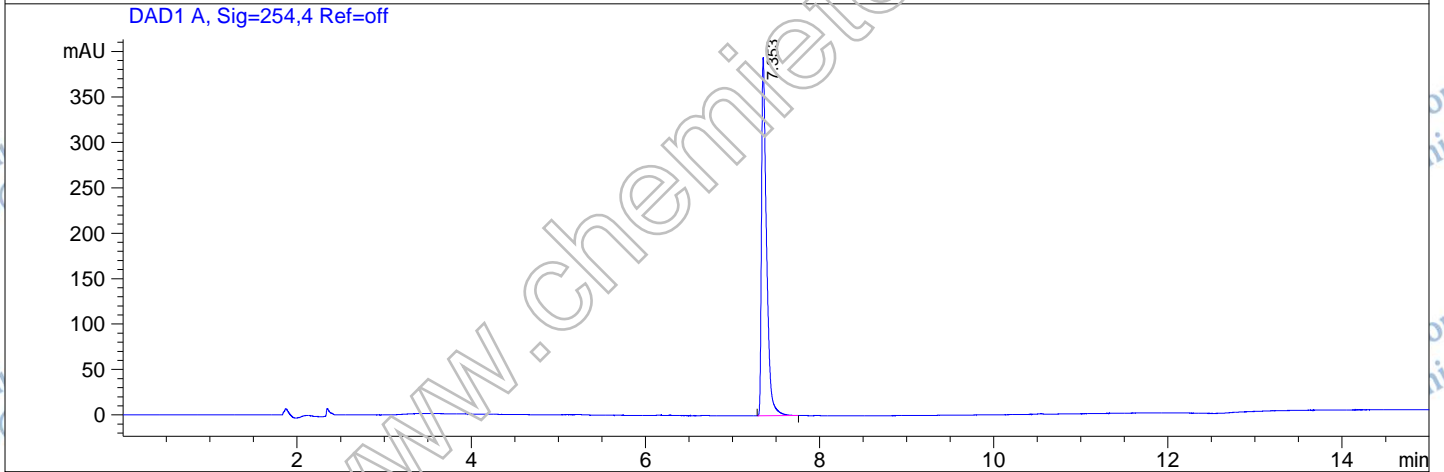


File ..T64\PRODUCT\SP-0017755-BAY2-11272-LCMS040.D Tgt Mass (EZ):
 Injection Date : 06-Dec-17, 22:25:00 Seq. Line : 0
 Sample Name : BAY-1816032 CHEMIETEK Lot 01 Location : P2-C-03
 Acq. Operator : 64product Inj : 0
 Spec. Reported : MS Integration Inj Volume : 5 ul
 Acq. Method : C:\Chem32\1\METHODS\HPLC-A.M
 Analysis Method : C:\CHEM32\1\METHODS\HPLC-A.M
 Sample Info : Easy-Access Method: 'HPLC-A.M'
 Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;
 Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;
 Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;
 Flow Rate: 1.0 mL/min;
 Column Temperature: 40 °C

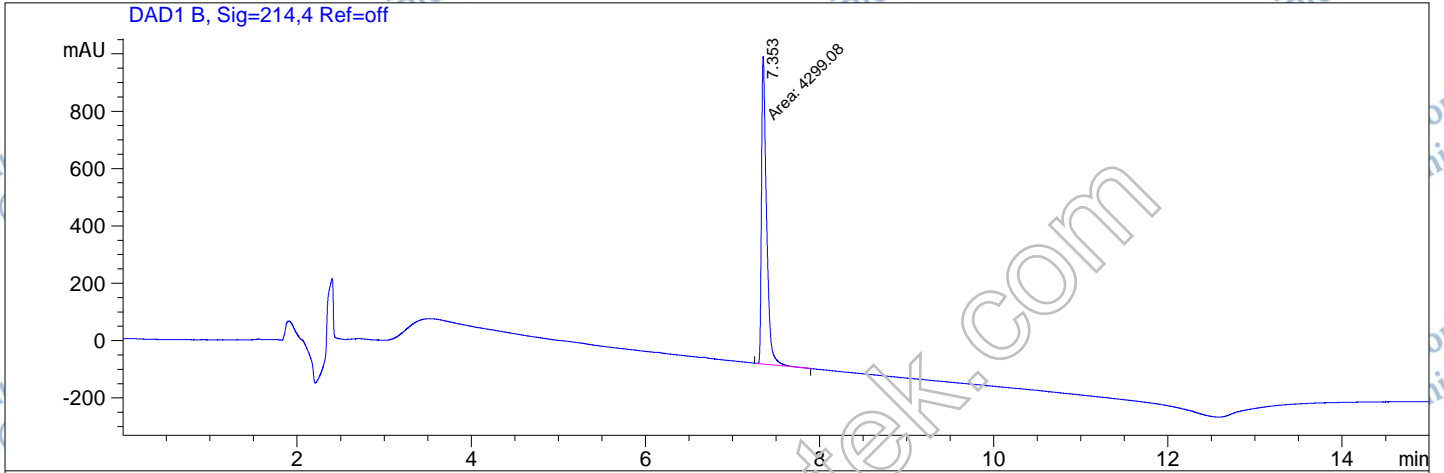

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.35	0.07	4299.08	1095.15	100.00

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.35	0.06	1577.18	394.63	100.00

