CHEMIETEK Chiral HPLC Report

Injection Date Time Stamp	14-04-24 8:47:51 PM
Injection Volume	3
Co-Solvent	
Column	
Sample	BIBW-2992-03
Sample Well	P1: 7A
Column Temperature	40
CO2 Flow Rate	2.4
Co-Solvent Flow Rate	0.6
Co-Solvent %	20
Back Pressure	120
Total Flow	3
PDA Start Wavelength	214
PDA Stop Wavelength	359
Injection Info	

Number	RT (min)	Area	Area %	Theoretical Plate
1	5.67	11717.8095	100	4043.8618

Peak Info

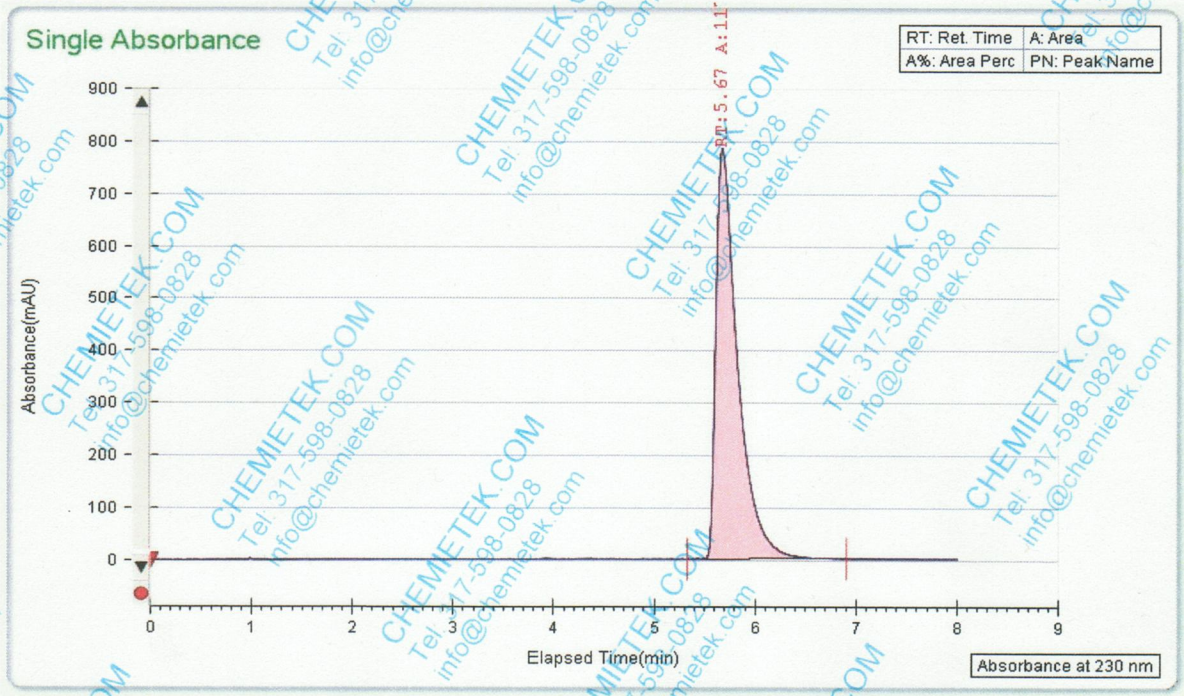

CHEMIETEK.COM
Tel: 317-598-0828
info@chemietek.com