

CHEMIETEK HPLC/MS Report

File D:\DATA\A02\MONITOR\CO-0826-2-01930-LCMSA036.D

Injection Date : 28 Aug 14 9:44 am +0800

Tgt Mass (EZS) :

Sample Name : CO-1686-02

Location : P2-A-01

Acq. Operator : A02-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 1 ul

Acq. Method : D:\METHODS\1-POS-3MIN.M

Analysis Method : D:\METHODS\1-POS-3MIN.M

Sample Info : Easy-Access Method: '1-POS-3MIN'


Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5%B increase to 95%B within 1.2min,
95%B for 1.3min, back to 5%B within 0.01min.

Flow Rate: 2.0 mL/min

Column: SunFire C18, 4.6*50mm, 3.5um

Column Temperature: 50 C

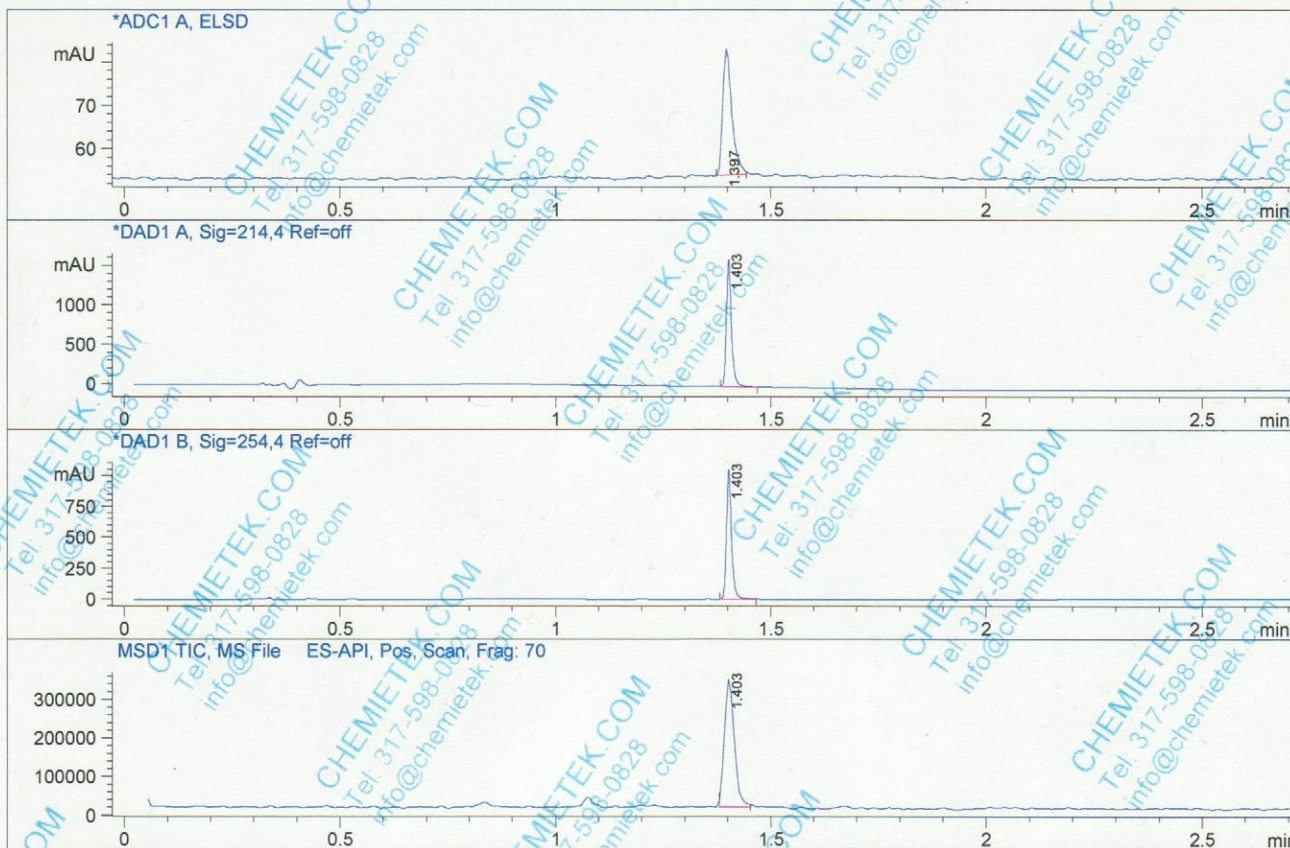

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.40	0.02	43.43	29.11	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.40	0.01	1364.27	1608.67	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.40	0.01	896.18	1020.04	100.00

CHEMIETEK HPLC/MS Report

Ret. Time: 1.40

<<<< POSITIVE SPECTRA >>>>

