


CVT-6883 DMSO 400MHz

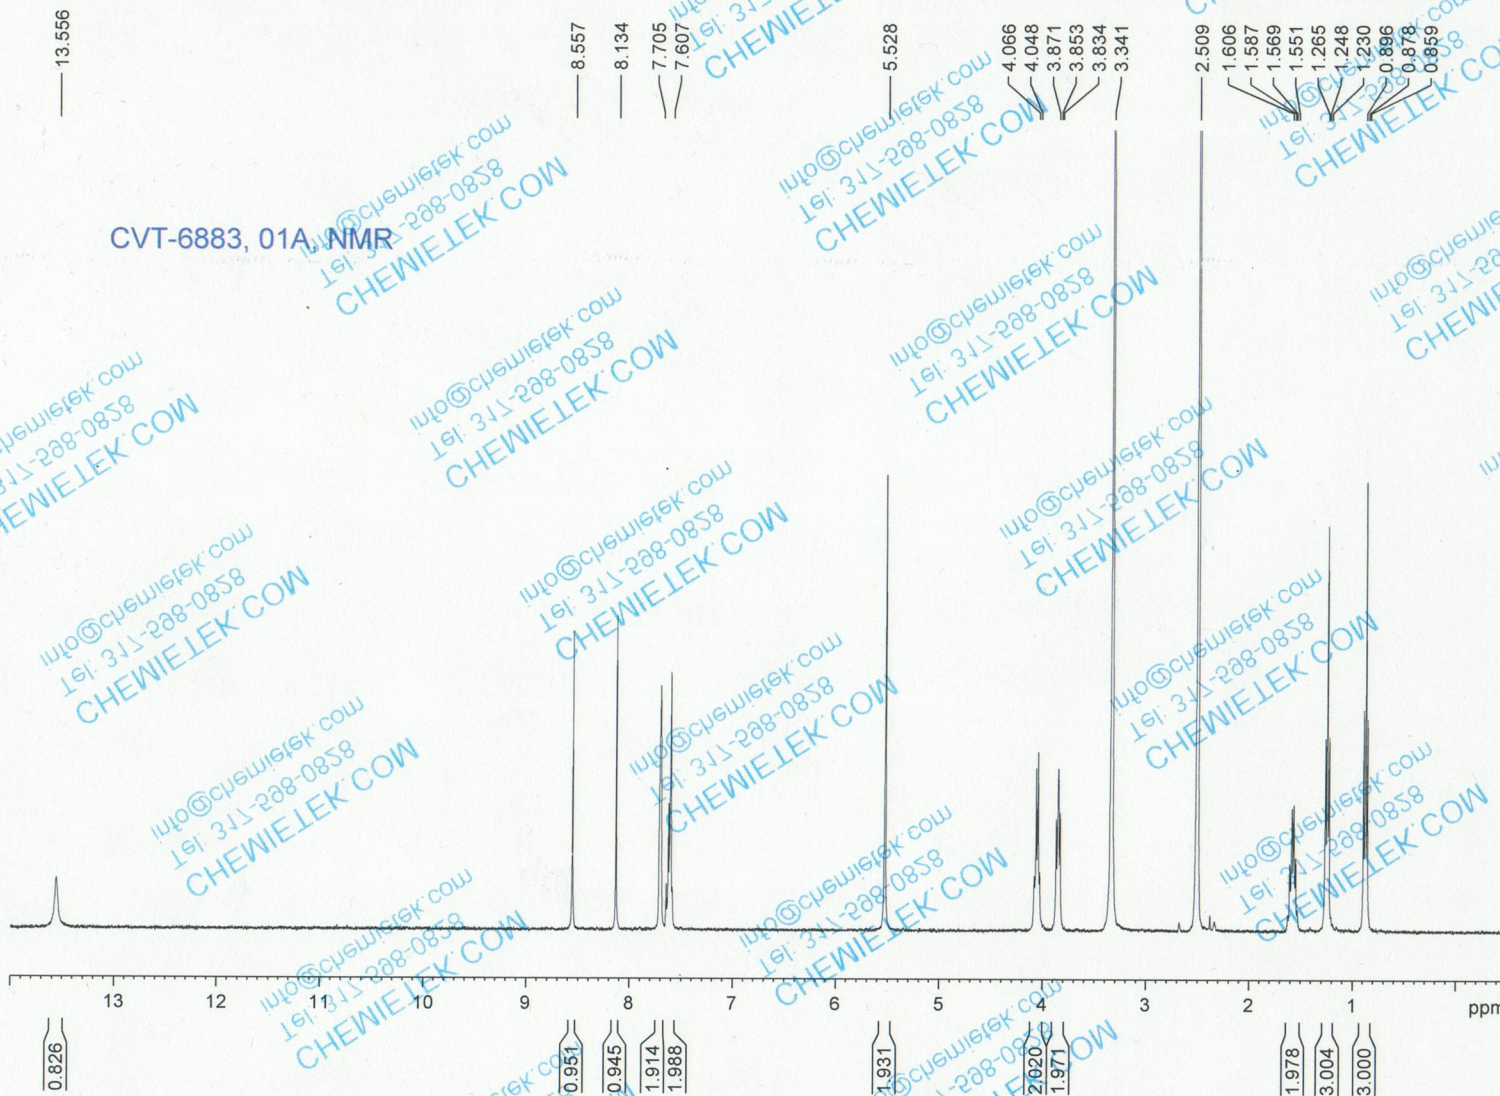

CVT-6883, 01A, NMR

Current Data Parameters
 NAME CVT-6883
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date 20121214
 Time 13.56
 INSTRUM Spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 65536
 SOLVENT DMSO
 NS 4
 DS 2
 SWH 8223.685 Hz
 FIDRES 0.125483 Hz
 AQ 3.9846387 sec
 RG 199.37
 DW 60.800 usec
 DE 6.50 usec
 TE 296.6 K
 D1 1.0000000 sec
 TD0 1

===== CHANNEL F1 =====
 NUC1 1H
 P1 13.50 usec
 PLW1 14.00000000 W
 SFO1 400.1324710 MHz

F2 - Processing parameters
 SI 65536
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00