


# CHEMIETEK Chiral HPLC Report




## Injection Info

Injection Date Time Stamp 6/22/2015 12:44:28 PM  
 Injection Volume 1  
 Co-Solvent  
 Column  
 Sample D-Single-5  
 Sample Well P1: 4C  
 Column Temperature 38.8  
 CO2 Flow Rate 2.55  
 Co-Solvent Flow Rate 0.45  
 Co-Solvent % 15  
 Total Flow 3  
 Front Pressure 172  
 Back Pressure 120  
 Pressure Drop 52  
 PDA Start Wavelength 214  
 PDA Stop Wavelength 359

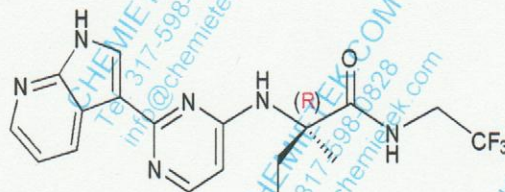

## Single Absorbance

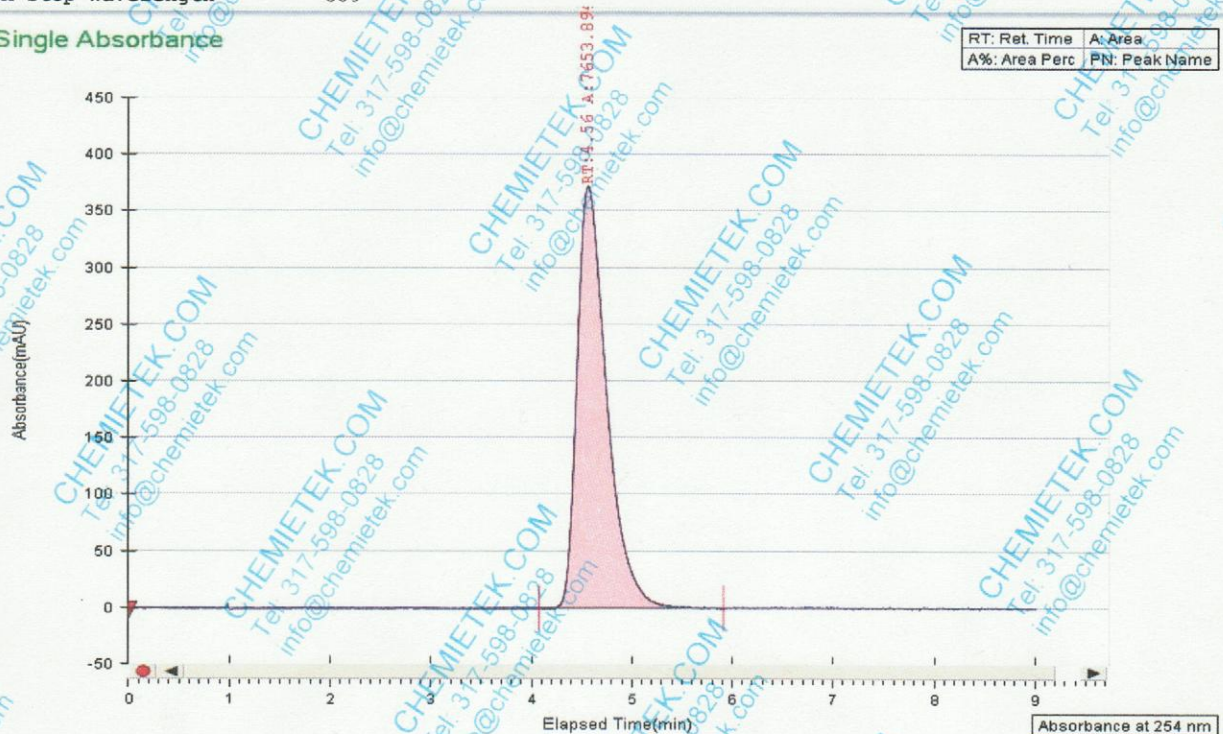


## Peak Info

Number	RT (min)	Area %	Area	Height
1	4.56	100	7653.8945	372.5028



CHEMIETEK HPLC/MS Report

File D:\DATA\A02\MONITOR\AC-20150305-7-17763-LCMSA002.D  
 Injection Date : 22 Jun 15 3:31 pm +0800 Tgt Mass (EZX) : 392.00  
 Sample Name : **Decernotinib-01** Location : P2-D-07  
 Acq. Operator : A02-MONITOR Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 2 ul  
 Acq. Method : D:\METHODS\1-POS-3MIN-MON.M  
 Analysis Method : D:\METHODS\1-POS-3MIN-MON.M  
 Sample Info : Easy-Access Method: '1-POS-3MIN-MON' 392.00  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5%B increase to 95%B within 1.6 min,  
 95%B for 1.4min,back to 5%B within 0.01min  
 Flow Rate:2.0ml/min  
 Column :SunFire C18, 4.6\*50mm, 3.5um  
 Oven Temperature : 50C

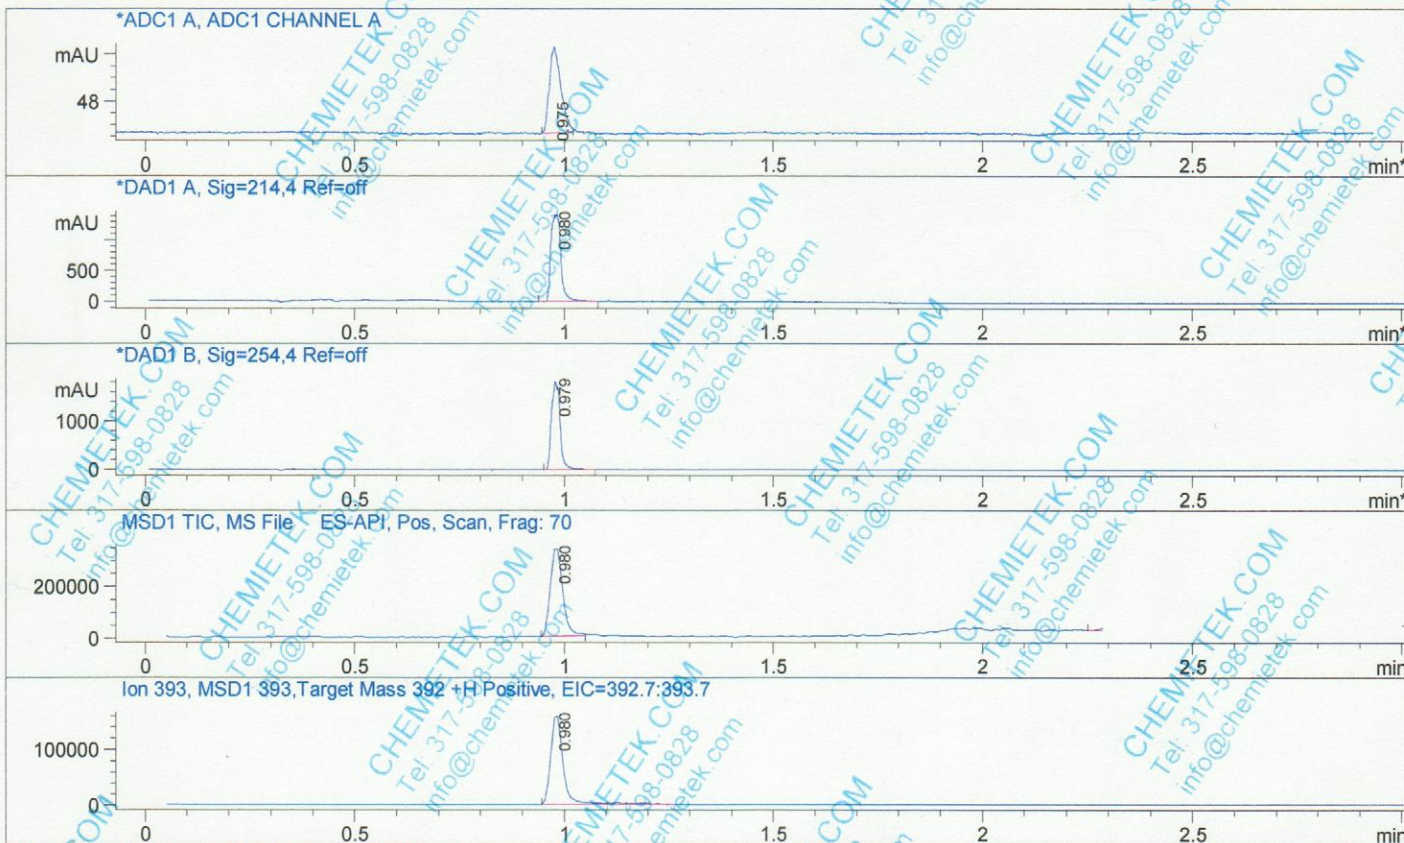


Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.98	0.03	2304.72	1398.96	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
0.98	0.02	2528.32	1744.03	100.00

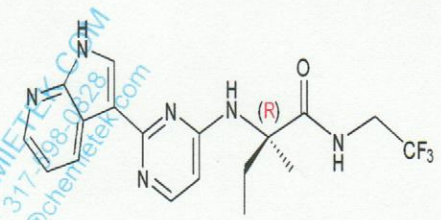

# CHEMIETEK HPLC/MS Report

Ret. Time: 0.98

<<<< POSITIVE SPECTRA >>>>

