CHEMIETEK HPLC/MS Report

```
File D:\DATA\A02\MONITOR\BFB-4-4-26785-LCMSA044.D
Injection Date    : 12 Sep 14  12:42 pm +0800       Tgt Mass(EZX) : 510.00
Sample Name       : CT-DEFA-01                          Location : P2-C-01
Acq. Operator     : A02-Monitor                            Inj : 1
Spec. Reported    : MS Integration                    Inj Volume : 1 ul
Acq. Method       : D:\METHODS\1-POS-3MIN.M
Analysis Method   : D:\METHODS\1-POS-3MIN.M
Sample Info : Easy-Access Method: '1-POS-3MIN'  510.00
Method Info : Mobile Phase: A:Water(10mM NH4HCO3)  B:ACN
              Gradient: 5% increase to 95%B within 1.4min,
                        95%B for 1.4min,back to 5%B within 0.01min
              Flow Rate: 1.8 ml/min
              Column: XBridge C18,4.6*50mm,3.5um
              Column Temperature: 50 C
```

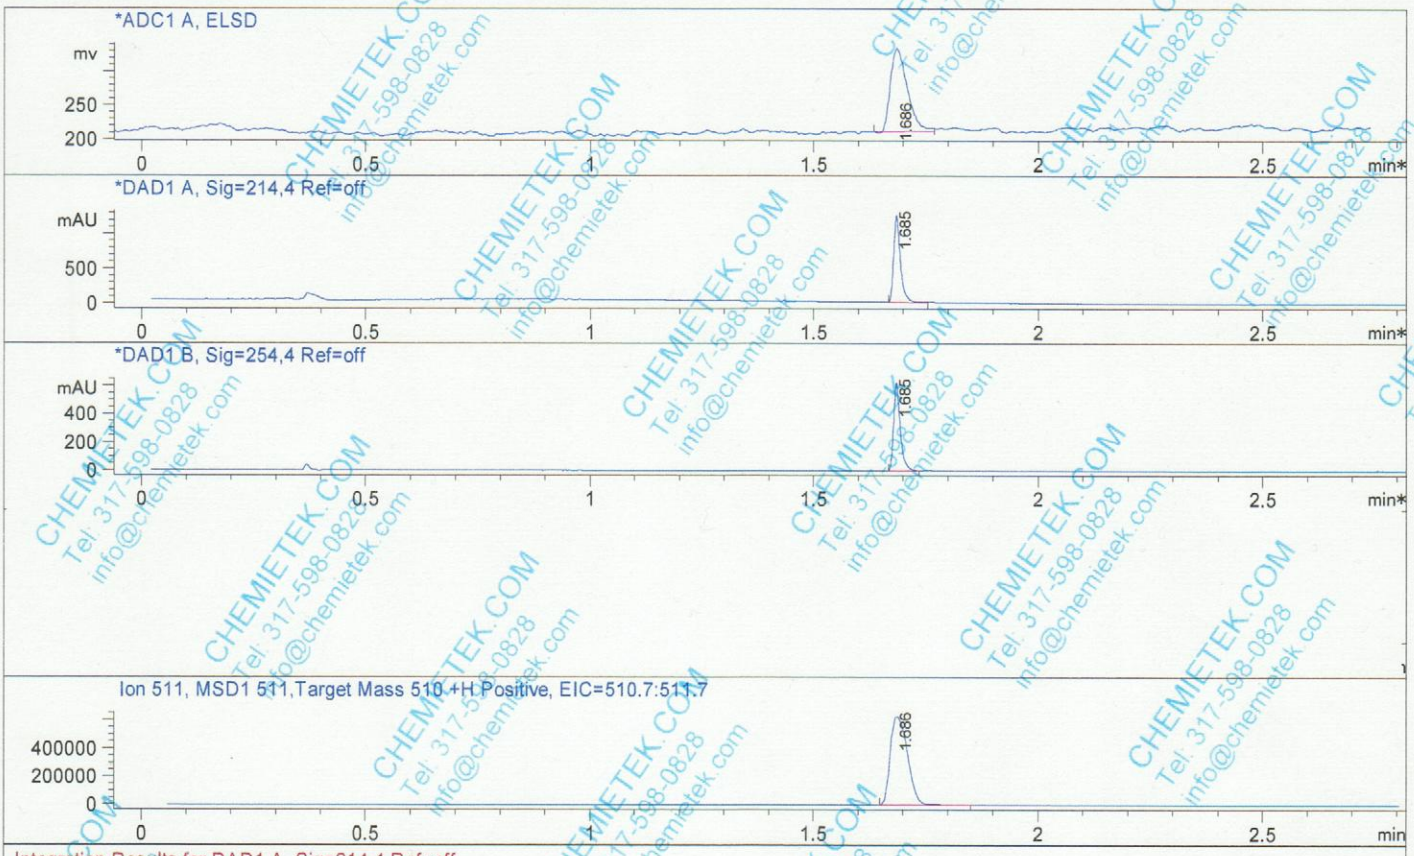


Integration Results for DAD1 A, Sig=214,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|---|---|---|---|---|
| 1.69 | 0.02 | 1302.73 | 1242.66 | 100.00 |

Integration Results for DAD1 B, Sig=254,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|---|---|---|---|---|
| 1.69 | 0.02 | 645.56 | 619.67 | 100.00 |

CHEMIETEK.COM Tel: 317-598-0828 info@chemietek.com

CHEMIETEK HPLC/MS Report

Ret. Time: 1.69 <<<< POSITIVE SPECTRA >>>>

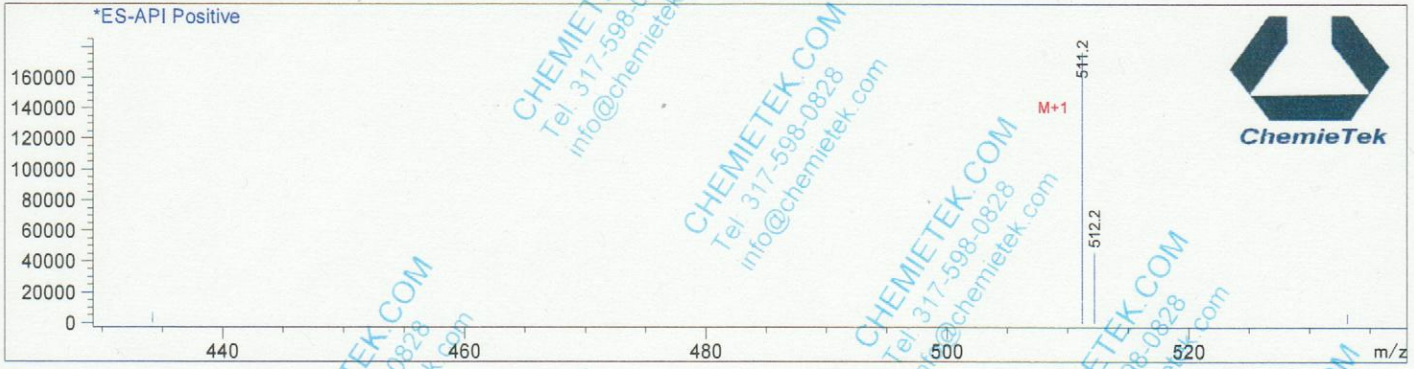


CHEMIETEK.COM
Tel: 317-598-0828
info@chemietek.com