



File ..UCT\SP-0017758-042-2-CHIRAL-13035-LCMS040.D Tgt Mass (EZ): 603.00
 Seq. Line : 0
 Sample Name : CT-LYC557 CHEMIETEK Lot 01 Location : P1-A-09
 Acq. Operator : 63product Inj : 1
 Spec. Reported : MS Integration Inj Volume : 3 ul
 Acq. Method : C:\Chem32\1\METHODS\HPLC-A-MS.M
 Analysis Method : C:\Chem32\1\METHODS\HPLC-A-MS.M
 Sample Info : Easy-Access Method: 'HPLC-A-MS.M' 603.00
 Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;
 Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;
 Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;
 Flow Rate: 1.0 mL/min;
 Column Temperature: 40 °C

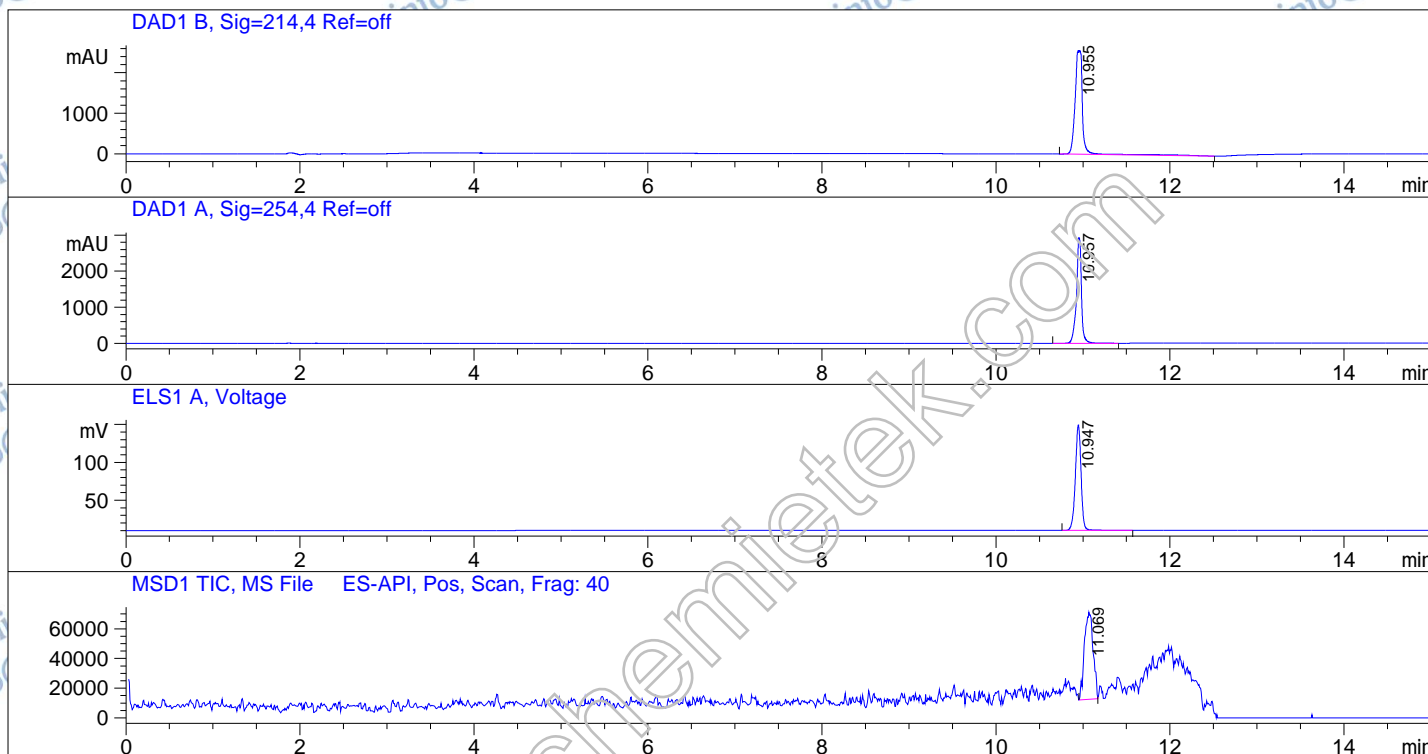

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
10.96	0.09	15581.53	2541.32	100.00

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
10.96	0.06	11663.33	2910.77	100.00

Integration Results for ELS1 A, Voltage

RetTim	Width	Area	Height	Area%
10.95	0.07	631.63	138.88	100.00

Ret. Time: 11.07

<<<< POSITIVE SPECTRA >>>>

