

File D:\DATA\CT06\MONITOR\FRAX486-04-68289-LCMSA040.D

Sample Name : FRAX486-04
Acq. Operator : 06monitor
Spec. Reported : MS Integration
Acq. Method : C:\CHEM32\1\METHODS\HPLC-A.M
Analysis Method : C:\CHEM32\1\METHODS\HPLC-A.M
Sample Info : Easy-Access Method: 'HPLC-A.M'
Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;
Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;
Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;
Flow Rate: 1.0 mL/min;
Column Temperature: 40 °C

Tgt Mass(EZX) :


Location : P1-F-08

Inj : 0


Inj Volume : 0.3 ul




ADC1 A, ADC1

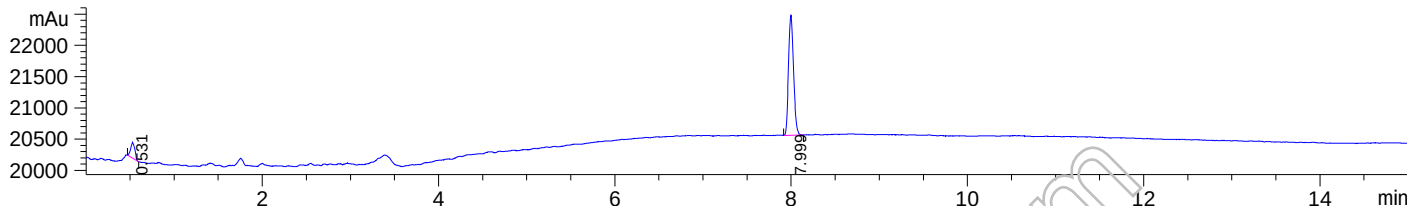



DAD1 A, Sig=254,4 Ref=off

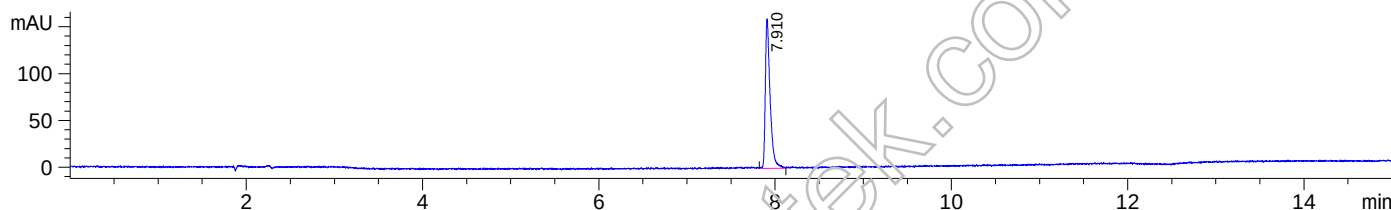

DAD1 B, Sig=214,4 Ref=off

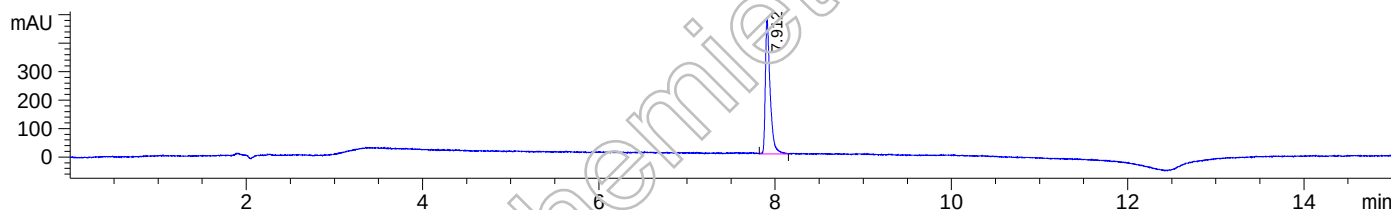

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 40

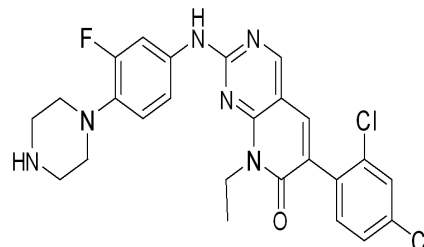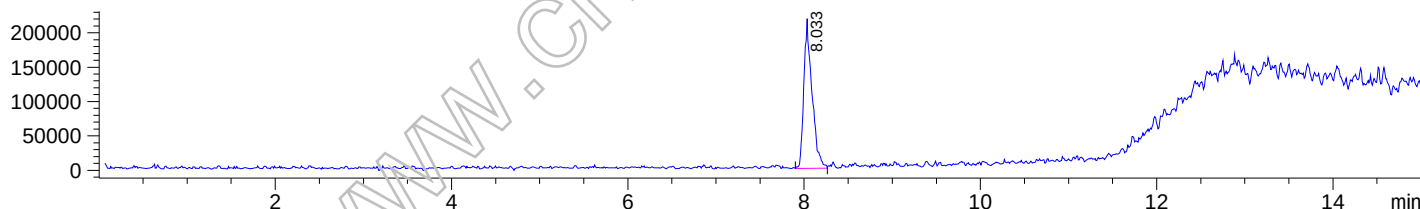

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.91	0.06	598.89	158.64	100.00

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.91	0.06	1774.70	455.37	100.00

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
--------	-------	------	--------	-------

Ret. Time: 8.03

<<<< POSITIVE SPECTRA >>>>

