

File ..\CT63\PRODUCT\ABBV-744-01-45159-LCMS040.D Tgt Mass (EZX): 491.00

Seq. Line : 0

Sample Name : ABBV-744 Lot 01

Location : P1-E-08

Acq. Operator : 63product

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 0.7 uL

Acq. Method : C:\Chem32\1\METHODS\HPLC-A-MS.M

Analysis Method : C:\CHEM32\1\METHODS\HPLC-A-MS.M

Sample Info : Easy-Access Method: 'HPLC-A-MS.M' 491.00


Method Info : Column: Waters X-Bridge C18: 150 mm*4.6 mm*3.5 um;

Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;

Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;

Flow Rate: 1.0 mL/min;

Column Temperature: 40 °C

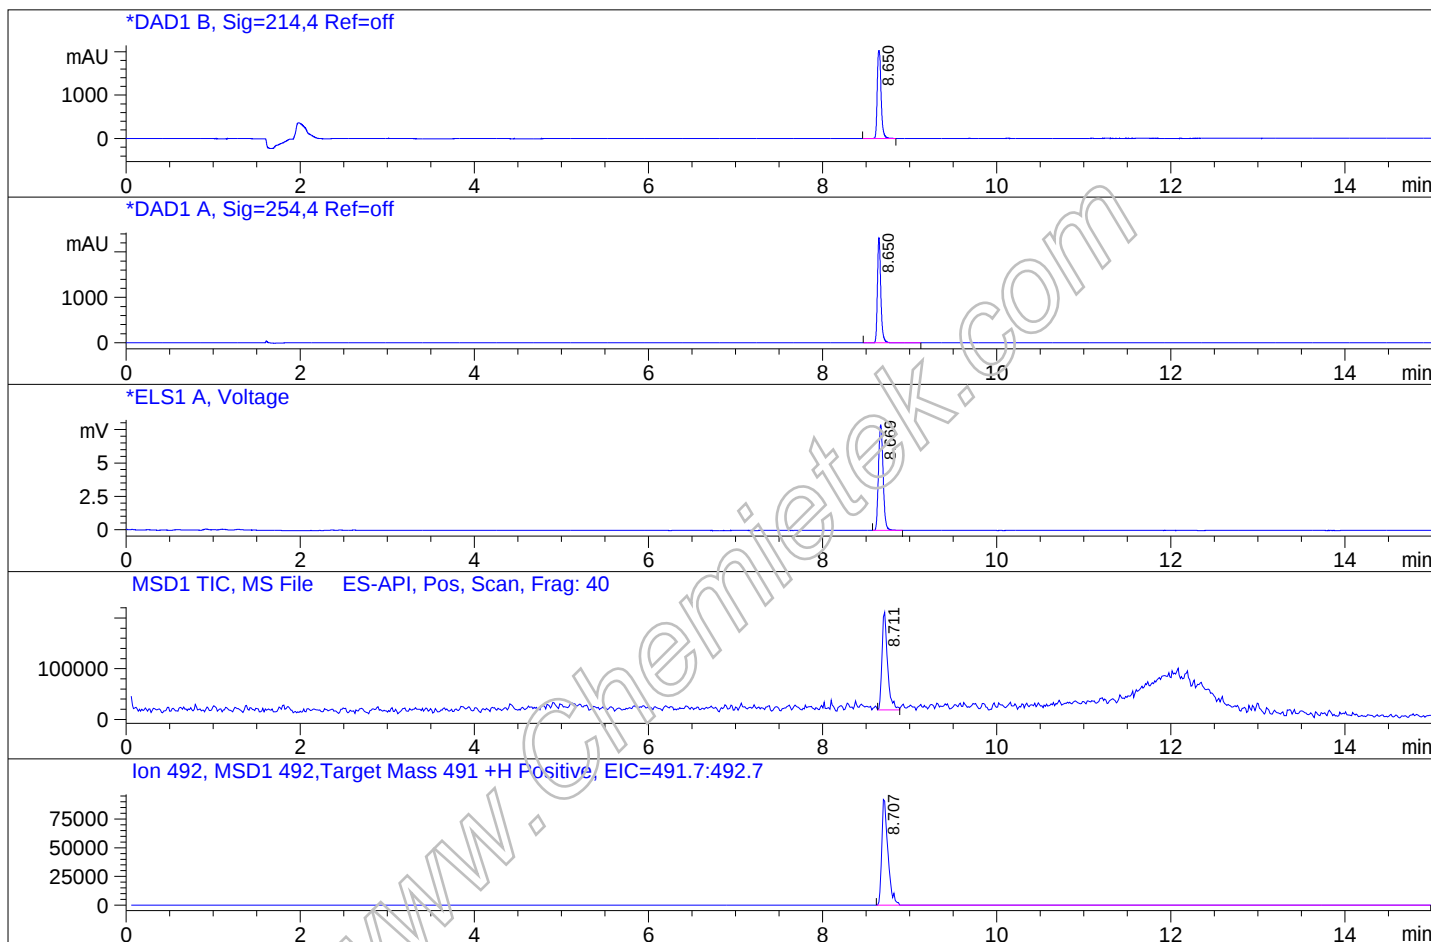

Integration Results for DAD1 B, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
8.65	0.05	6128.42	2019.55	100.00

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
8.65	0.04	6187.27	2299.79	100.00

Integration Results for ELS1 A, Voltage

RetTim	Width	Area	Height	Area%
8.67	0.06	29.25	7.89	100.00

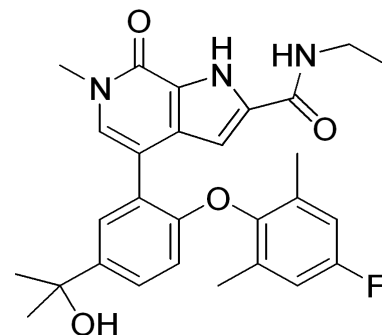

Ret. Time: 8.71

<<<< POSITIVE SPECTRA >>>>

