

=====


Acq. Operator : SYSTEM
Acq. Instrument : 1260

Seq. Line : 15
Location : 21



Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

Additional Info : Peak(s) manually integrated

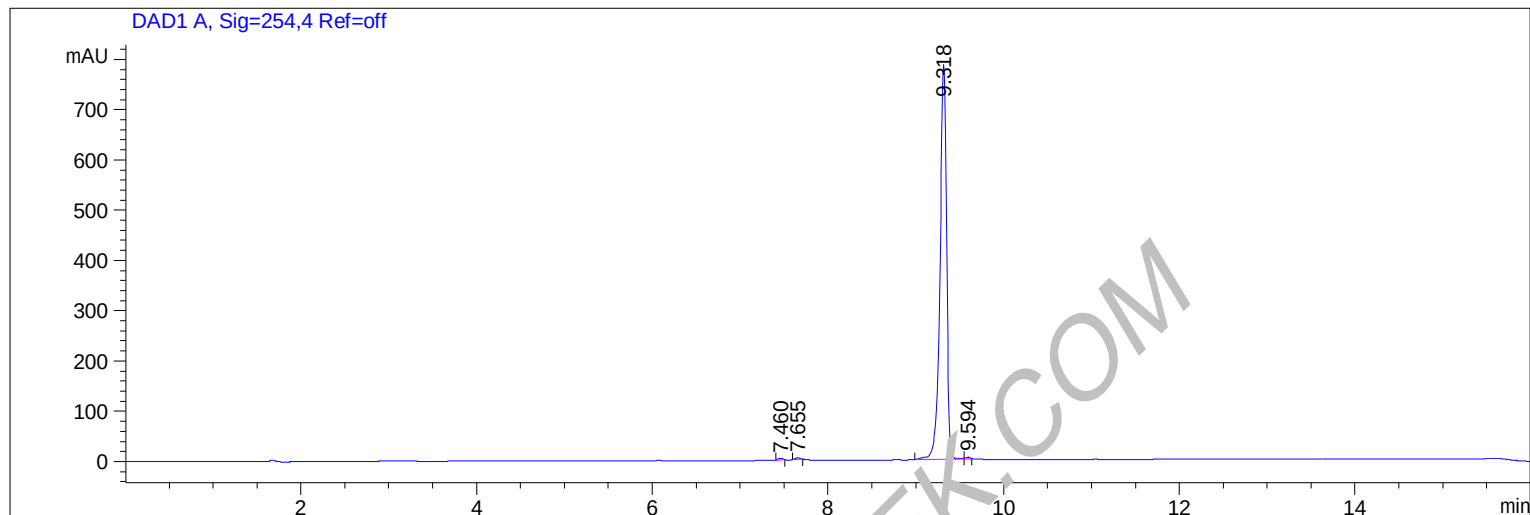


=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISiDs

Signal 1: DAD1 A, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	7.460	MM R	0.0590	11.04880	3.12058	0.2697
2	7.655	MM R	0.0675	12.47087	3.07826	0.3044
3	9.318	MF R	0.0861	4063.38062	786.89941	99.1767
4	9.594	FM R	0.0623	10.21262	2.73253	0.2493

Totals : 4097.11290 795.83078

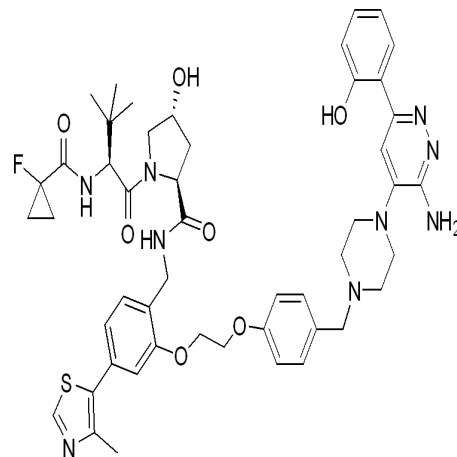

=====
*** End of Report ***