



HPLC Analysis Report

Sample name: ADU-S100, Lot 03




Acquired on: Default

Instrument: LCMS-080

Acq. method: T3_0-30LAB_20min.amx

Location: D1F-C6

Injection Data File Directory /data/IT/Results/LC_MS-080/Default.rslt

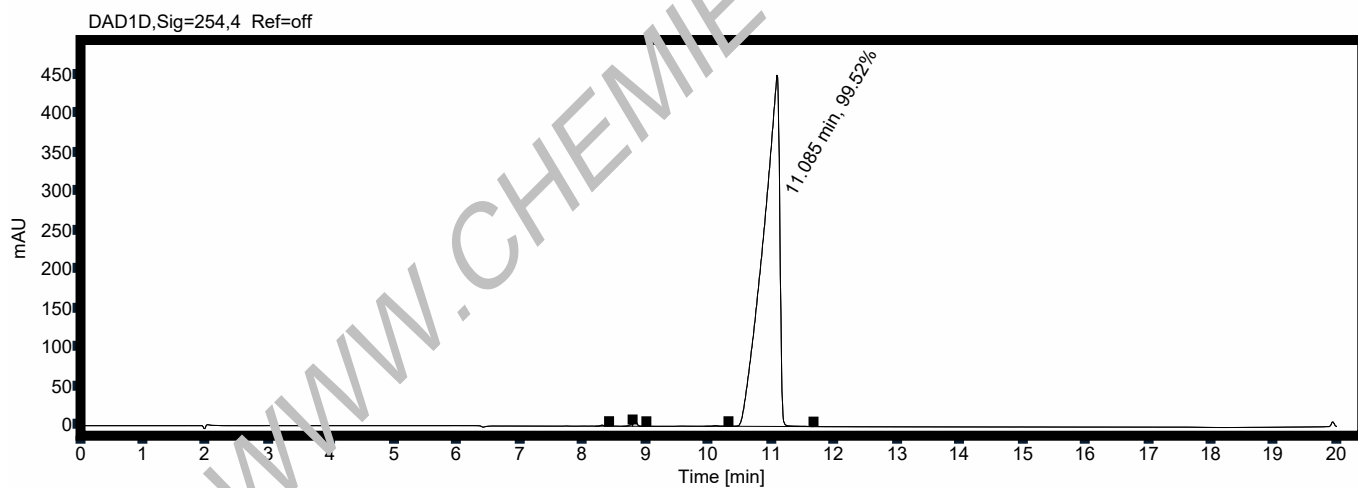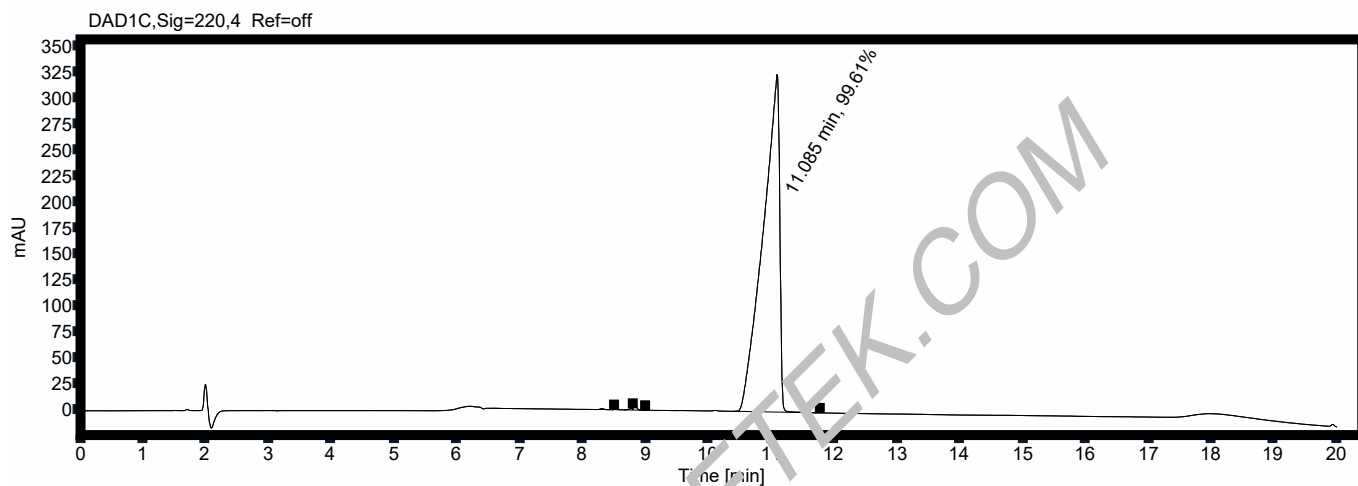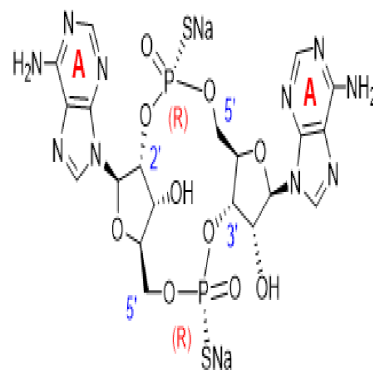

Signal: DAD1C,Sig=220,4 Ref=off

RT [min]	Height	Width	Area	Area%
8.299	0.90	0.33	2.67	0.04
8.785	1.48	0.14	5.52	0.09
8.830	3.91	0.20	14.86	0.25
11.085	323.78	1.37	5952.08	99.61

Signal: DAD1D,Sig=254,4 Ref=off

RT [min]	Height	Width	Area	Area%
8.299	1.32	0.22	5.03	0.06
8.785	2.20	0.16	8.00	0.10
8.830	5.75	0.22	22.25	0.27
10.105	0.76	0.38	4.80	0.06
11.085	449.57	1.35	8246.58	99.52