






# HPLC Analysis Report

**Sample name:** ADU-S100, Lot 03  
**Acquired on:** Default  
**Instrument:** LCMS-080  
**Acq. method:** T3\_0-30LAB\_20min.amx  
**Location:** D1F-C6

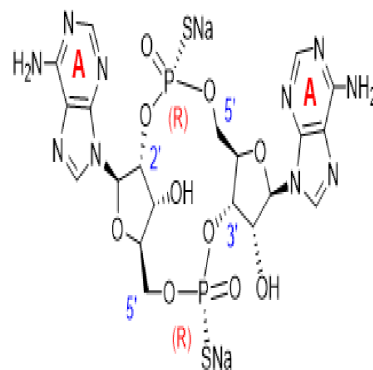

**Injection Data File Directory** /data/IT/Results/LC\_MS-080/Default.rslt

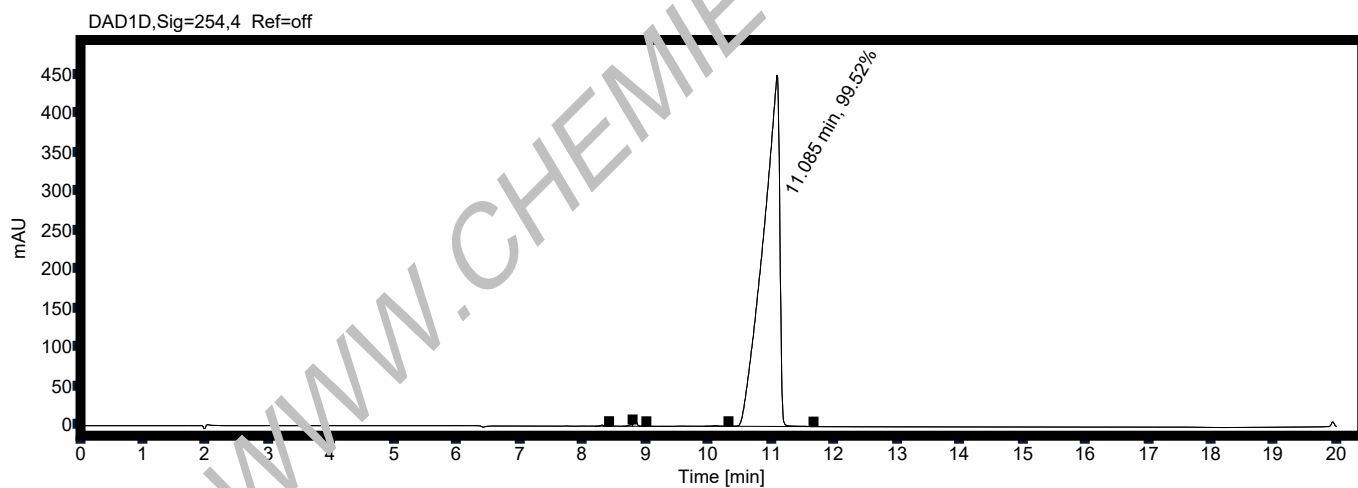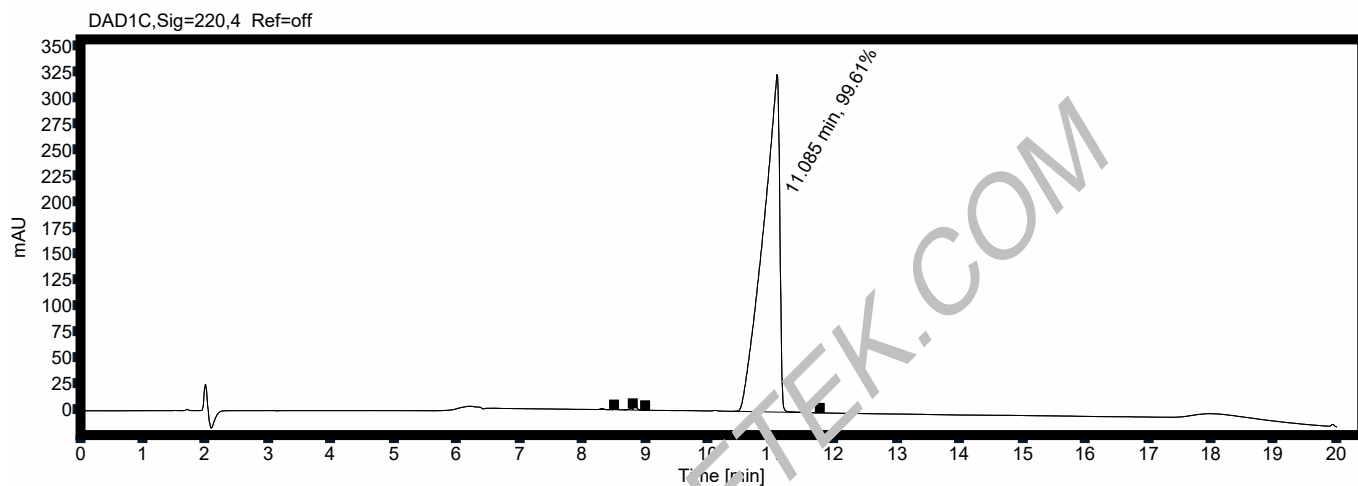

**Signal:** DAD1C,Sig=220,4 Ref=off

| RT [min] | Height | Width | Area    | Area% |
|----------|--------|-------|---------|-------|
| 8.299    | 0.90   | 0.33  | 2.67    | 0.04  |
| 8.785    | 1.48   | 0.14  | 5.52    | 0.09  |
| 8.830    | 3.91   | 0.20  | 14.86   | 0.25  |
| 11.085   | 323.78 | 1.37  | 5952.08 | 99.61 |

**Signal:** DAD1D,Sig=254,4 Ref=off

| RT [min] | Height | Width | Area    | Area% |
|----------|--------|-------|---------|-------|
| 8.299    | 1.32   | 0.22  | 5.03    | 0.06  |
| 8.785    | 2.20   | 0.16  | 8.00    | 0.10  |
| 8.830    | 5.75   | 0.22  | 22.25   | 0.27  |
| 10.105   | 0.76   | 0.38  | 4.80    | 0.06  |
| 11.085   | 449.57 | 1.35  | 8246.58 | 99.52 |