



File D:\DATA\ADMIN\MONITOR\AZD8421-008-H-98487-LCMSA001.D




Sample Name : AZD8421 Lot 01
Acq. Operator : ADMIN
Spec. Reported : MS Integration
Acq. Method : D:\METHODS\1-CHEMIELAB-HPLC-3MIN.M
Analysis Method : D:\METHODS\1-CHEMIELAB-HPLC-3MIN.M
Sample Info : CHEMIELAB HPLC Method: '1-CHEMIELAB-HPLC-3MIN.M'
Method Info : Default Method

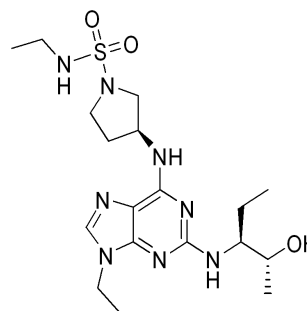


*DAD1 A, Sig=214,4 Ref=off

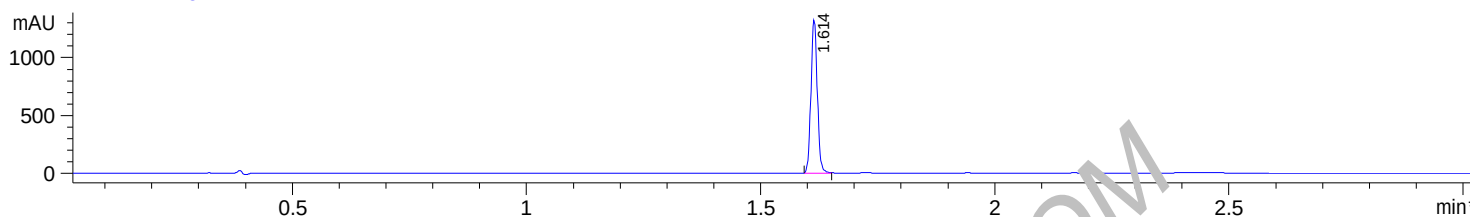


*DAD1 B, Sig=254,4 Ref=off

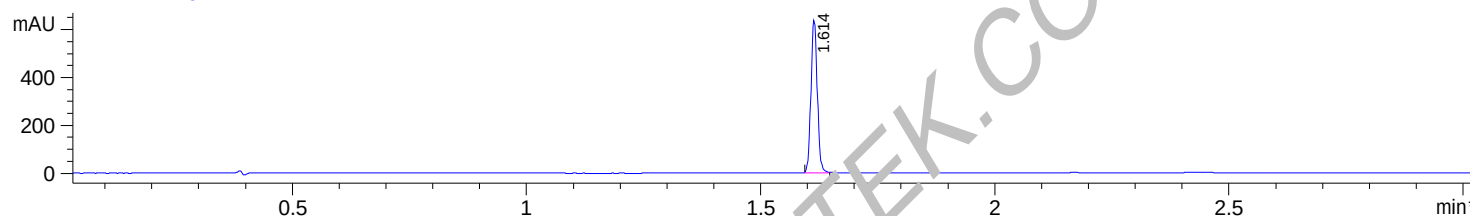

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 100

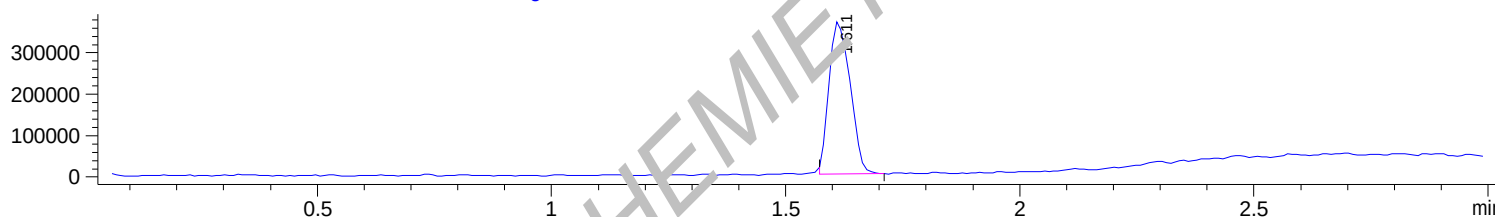

Ion 441, MSD1 441, Target Mass 440 +H Positive, C1C 440.7:441.7

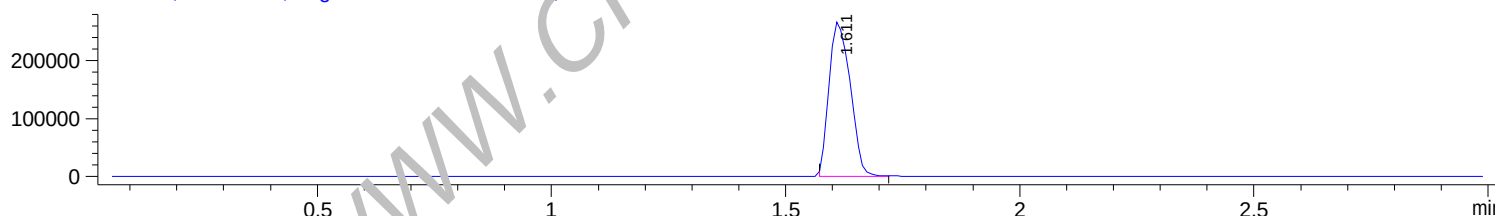

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.61	0.01	1246.15	1322.99	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.61	0.01	599.88	637.29	100.00

Ret. Time: 1.61

<<<< POSITIVE SPECTRA >>>>

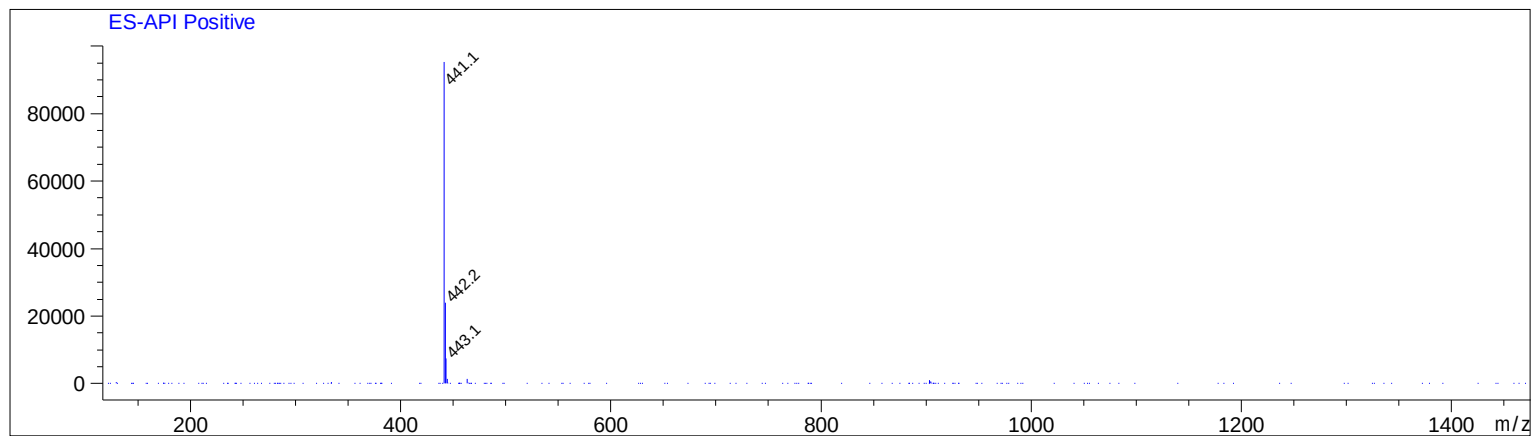

WWW.CHEMIETEK.COM