

Sample Name : CT-AZD3458 01

Acq. Operator : C52-MONITOR

Spec. Reported : MS Integration

Acq. Method : D:\METHODS\2-HPLC-15MIN.M

Analysis Method : D:\METHODS\2-HPLC-15MIN.M

Sample Info : Easy-Access Method: '2-HPLC.M'

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.

Flow Rate: 1.0ml/min

Column:Sunfire C18,4.6*150mm,3.5um

Column Temperature: 45 C

Tgt Mass(EZX) :


Location : P1-D-07

Inj : 0


Inj Volume : 3 ul



DAD1 A, Sig=214,4 Ref=off

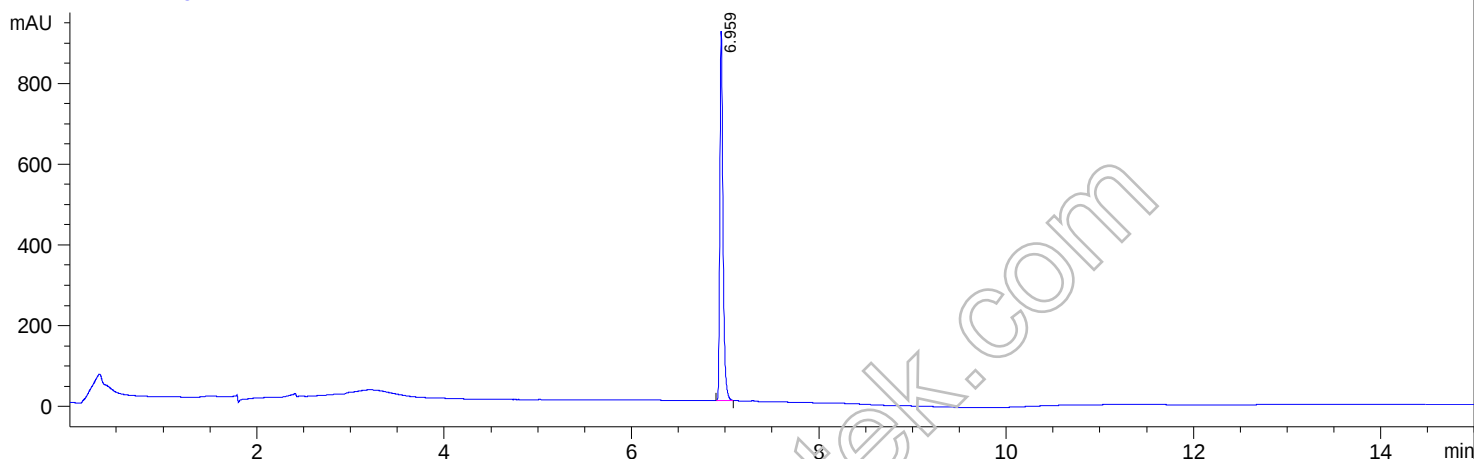

DAD1 B, Sig=254,4 Ref=off

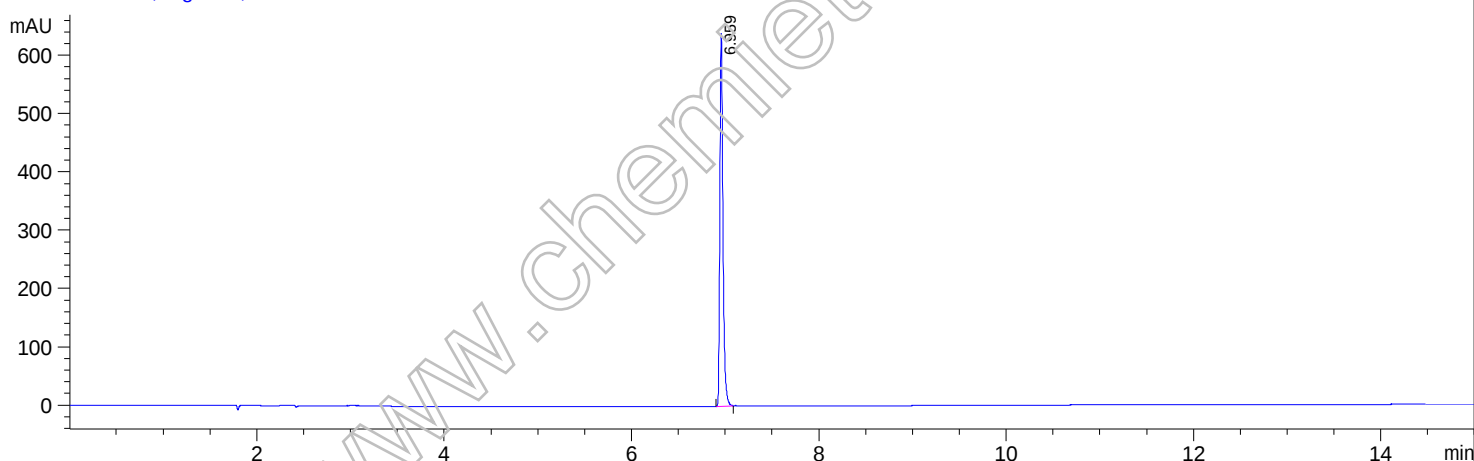

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
6.96	0.03	2086.52	915.56	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.96	0.03	1446.85	639.68	100.00

