Data File D:\DATA\Default\CT-LY283M-01\Online.D
Sample Name: CT-LY283M-01

==========

Acq. Operator : SYSTEM Seq. Line : 6
Acq. Instrument : HPLC1260

Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

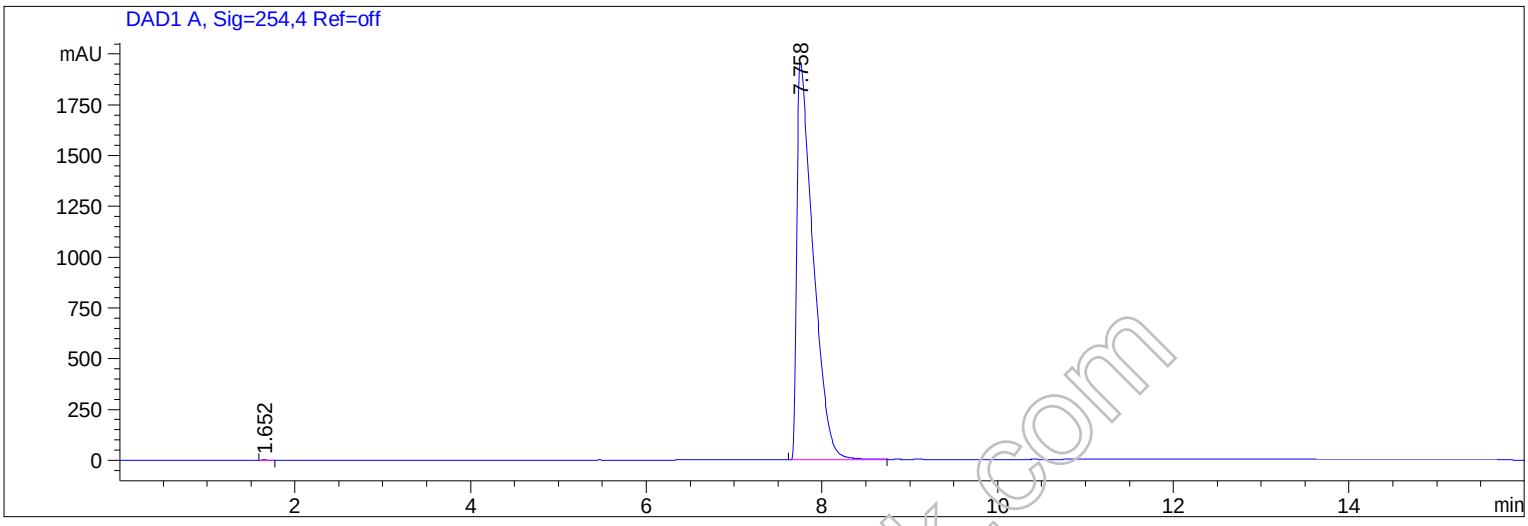

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

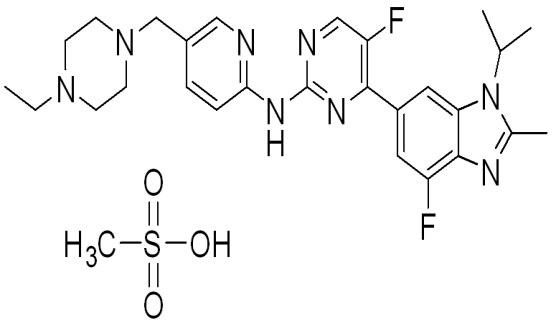

Signal 1: DAD1 A, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.652	BV	0.0642	16.69747	3.88205	0.0659
2	7.758	BB	0.1870	2.53228e4	1956.14758	99.9341

Totals : 2.53395e4 1960.02963

==========

*** End of Report ***

www.chemietek.com