

File ..T64\PRODUCT\SP-0017755-BAY2-11272-LCMS040.D Tgt Mass (EZ):

Sample Name : BAY-1816032 CHEMIETEK Lot 01

Acq. Operator : 64product

Spec. Reported : MS Integration

Acq. Method : C:\Chem32\1\METHODS\HPLC-A.M

Analysis Method : C:\CHEM32\1\METHODS\HPLC-A.M

Sample Info : Easy-Access Method: 'HPLC-A.M'

Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;

Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;

Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;

Flow Rate: 1.0 mL/min;

Column Temperature: 40 °C

Seq. Line : 0


Location : P2-C-03

Inj : 0


Inj Volume : 5 uL



DAD1 B, Sig=214,4 Ref=off

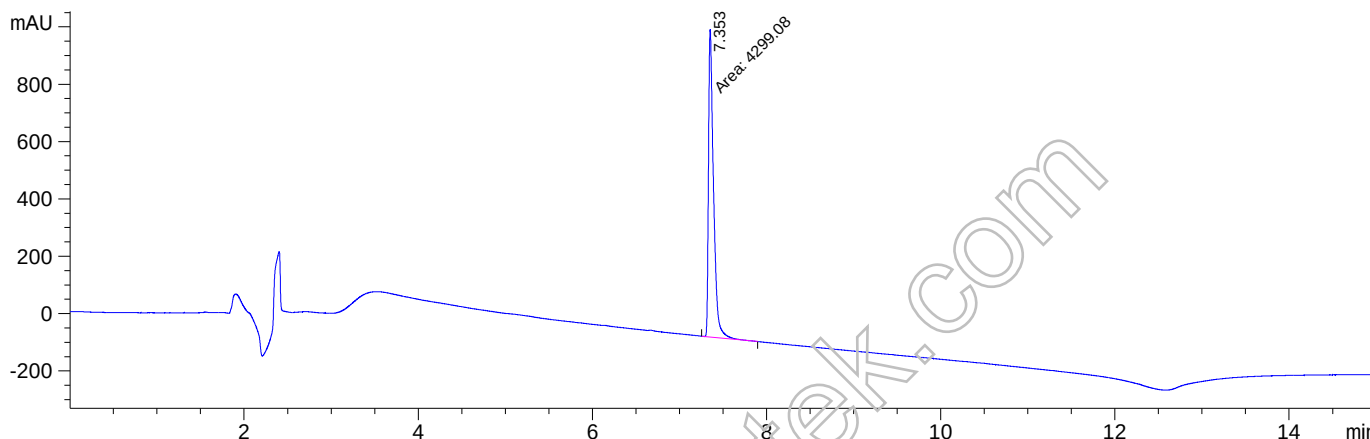

DAD1 A, Sig=254,4 Ref=off

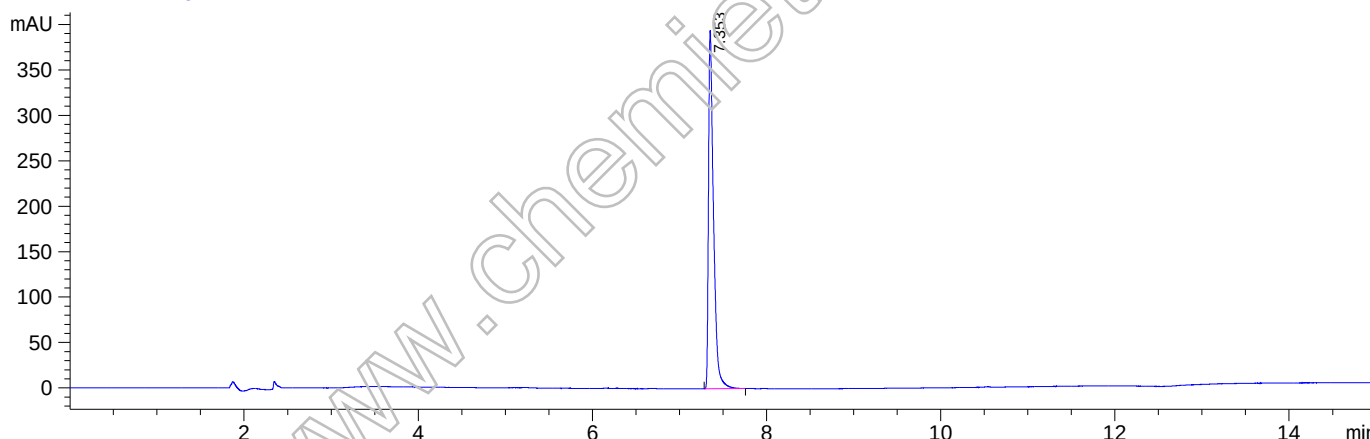

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.35	0.07	4299.08	1095.15	100.00

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.35	0.06	1577.18	394.63	100.00

