

File D:\DATA\C52\MONITOR\BAY-293-23232-LCMSA013.D

Sample Name : BAY-293

Acq. Operator : C52-MONITOR

Spec. Reported : MS Integration

Acq. Method : D:\METHODS\2-POS-15MIN.M

Analysis Method : D:\METHODS\2-POS-15MIN.M

Sample Info : Easy-Access Method: '2-POS-15MIN' 448.00

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.

Flow Rate: 1.0ml/min

Column: Sunfire C18, 4.6*150mm, 3.5um

Column Temperature: 45 C


Detection: UV(214,4nm) and MS(ESI, Pos mode, 110 to 1500 amu)

Tgt Mass(EZX) : 448.00

Location : P1-C-08

Inj : 1

Inj Volume : 1 ul

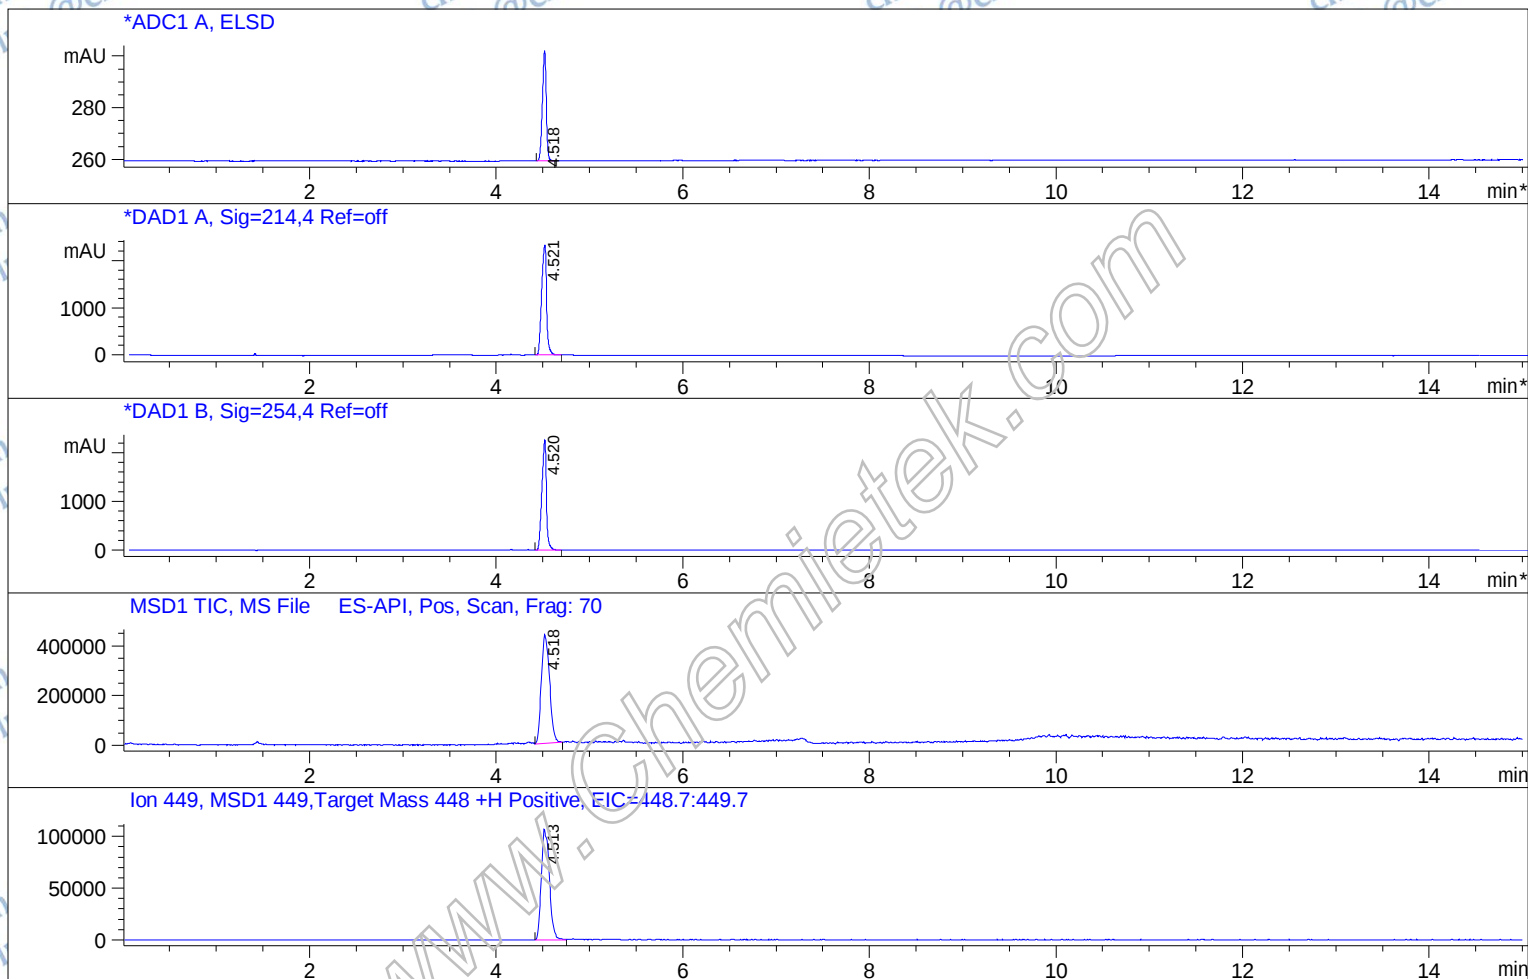

Integration Results for ADC1 A, ELSD


RetTim	Width	Area	Height	Area%
4.52	0.04	122.40	42.63	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
4.52	0.06	8578.75	2326.39	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
4.52	0.05	7631.76	2263.75	100.00

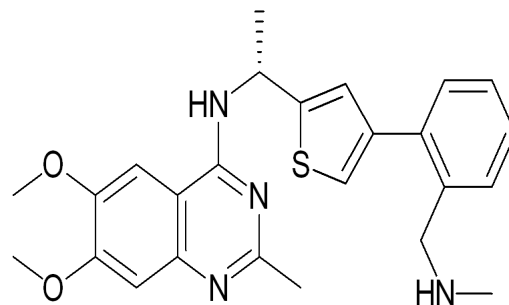

Ret. Time: 4.52

<<<< POSITIVE SPECTRA >>>>

