CHEMIETEK Chiral HPLC Report

Injection Volume	5
Co-Solvent	
Column	AS-H (4.6*250mm, 5um)
Sample	CEP-28122-01
Sample Well	P1: 3F
Column Temperature	39.8
CO2 Flow Rate	1.95
Co-Solvent Flow Rate	1.05
Co-Solvent %	35
Back Pressure	120
Total Flow	3
PDA Start Wavelength	214
PDA Stop Wavelength	359

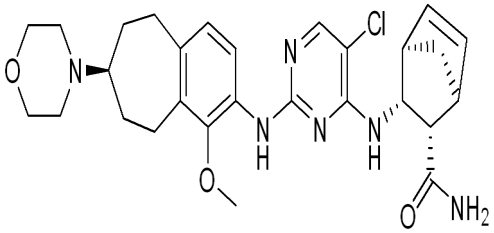

Injection Info

Number	RT (min)	Area	Area %	Theoretical Plate
1	3.71	6308.4337	100	3388.4792

Peak Info

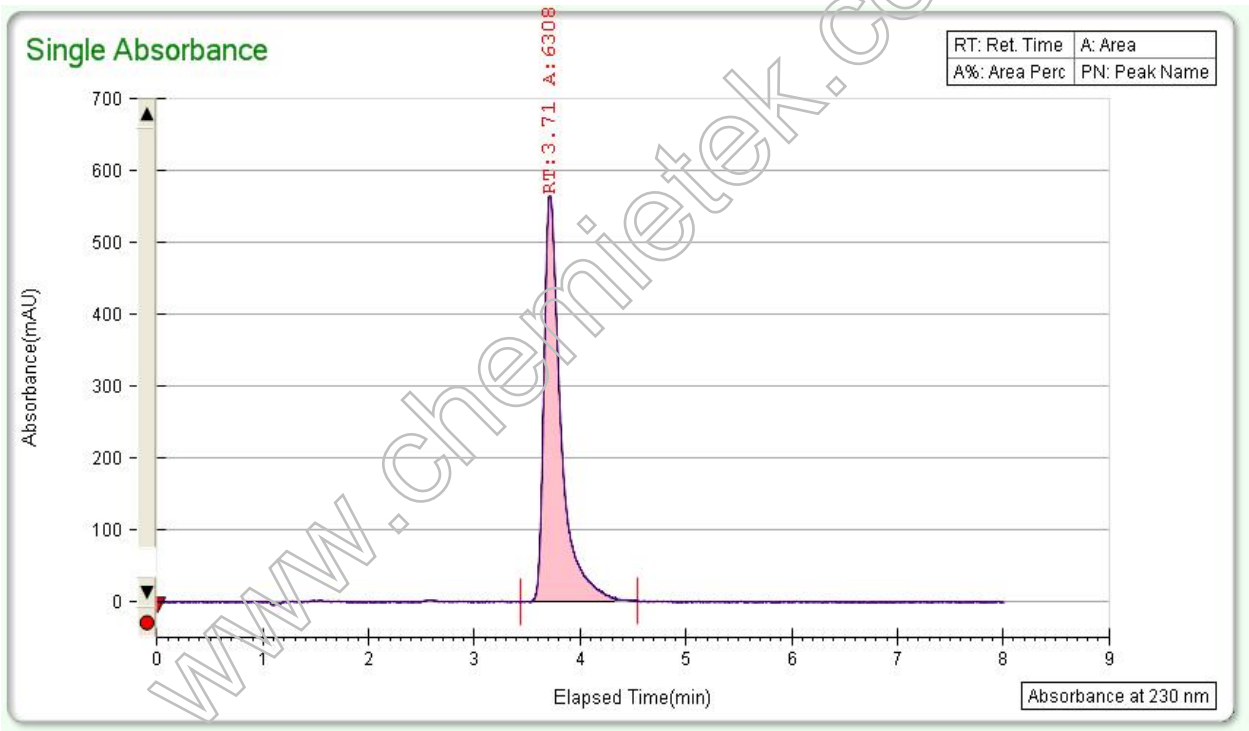

www.chemietek.com