





CHIRAL HPLC REPORT

SAMPLE INFORMATION

Sample ID: Default
Compound ID: GDC-1971, Lot 01
Acq Method: Default
Channel Name: PDA Ch1 220nm@4.8nm
Proc. Chnl. Descr.: PDA Ch1 220nm@4.8nm



Instrument: Waters UPCC with PDA Detector

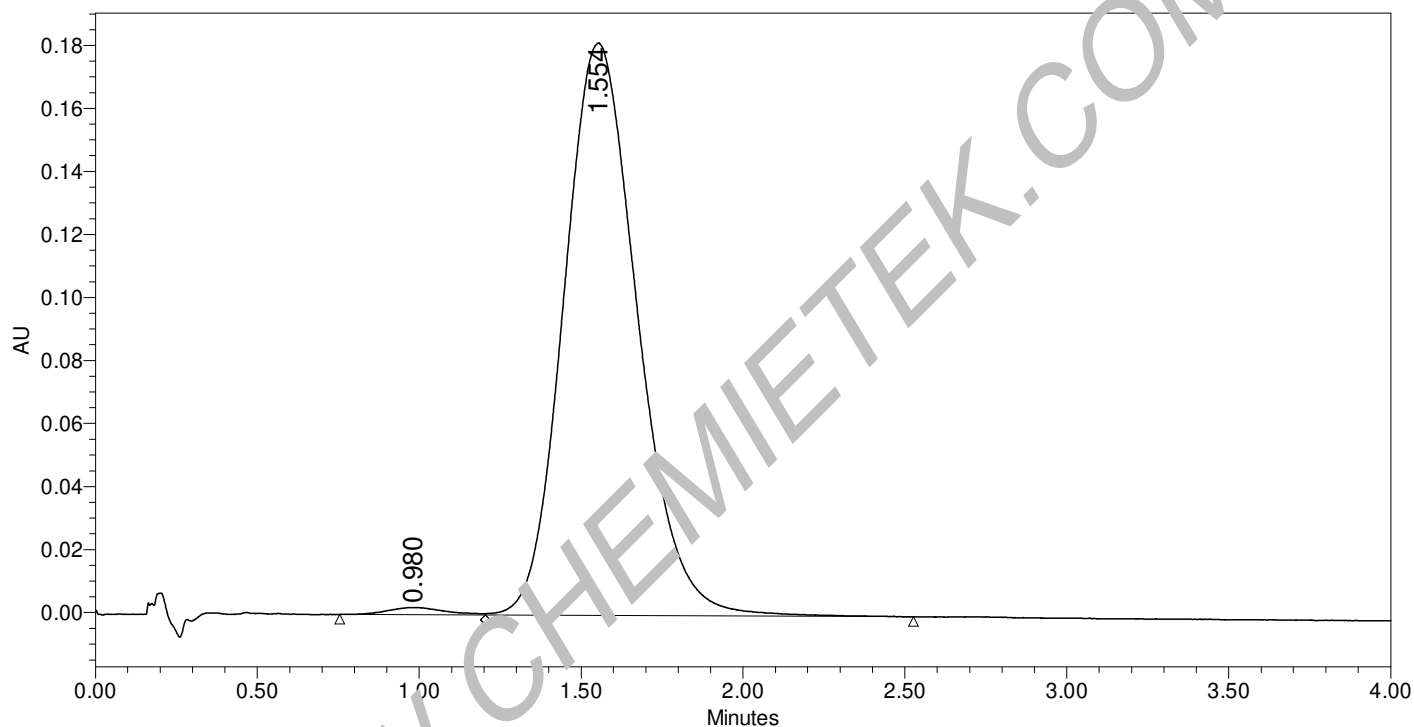

	RT	Area	% Area
1	0.980	28437	0.98
2	1.554	287328	99.02