



# Chiral HPLC Report

Sample : CT-G6036-Lot 1 (In Ethanol 1mg/mL)


Mobile Phase : 50%n-hexane/50%ethanol/0.1%DEA

Flow Rate : 1ml/min


Injection : 1 $\mu$ L

Detector : UV 254nm

Temperature : 25 °C

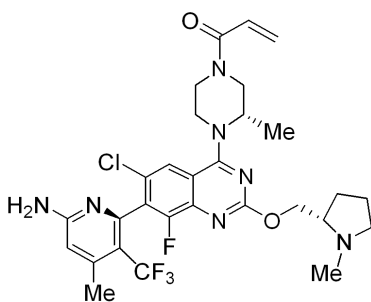

## Test Results:

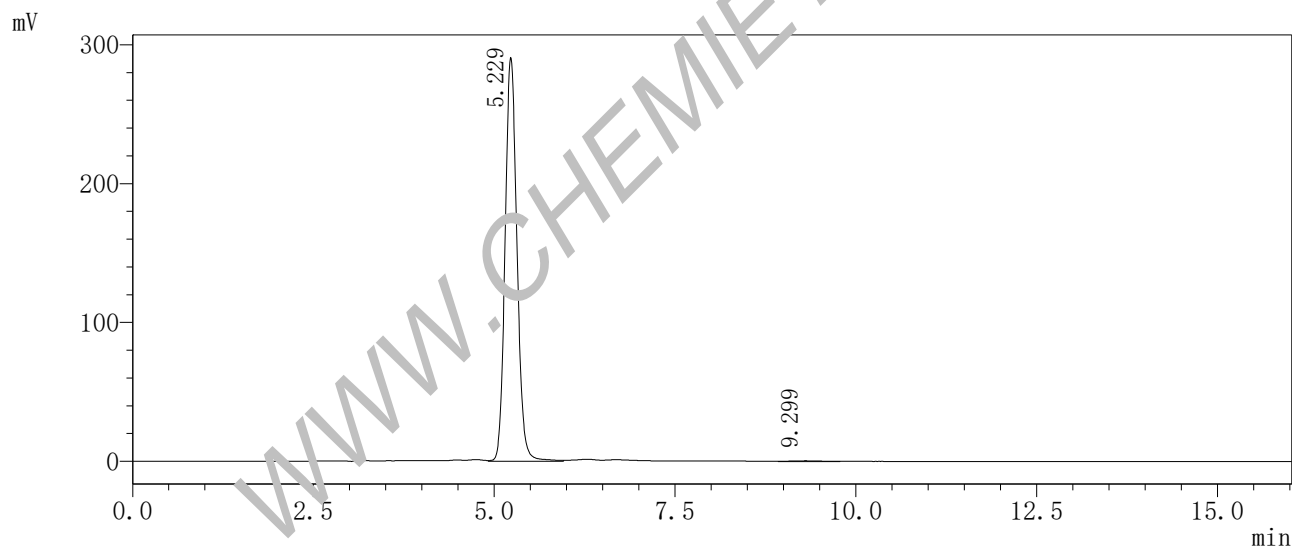

Ch1 254nm

S#	Retention Time	Height	Area%	Resolution	Tailing Factor
1	5.229	290852	99.586	--	1.113
2	9.299	471	0.414	7.751	--