






HPLC REPORT

<Sample Information>

Acquired by : Admin
Sample Name : GS-9688, Lot 01
Sample ID : CT-GS9688-01
Vial # : L-1
Injection Volume : 5 uL
Data File Name : CT-GS9688-01.cd
Method File Name : HPLC-18min.1cm
Batch File Name : Default
Report File Name : HPLC_18min.1cr

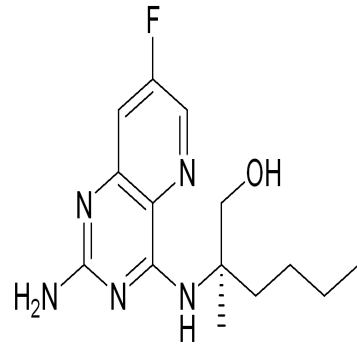

<Chromatogram>

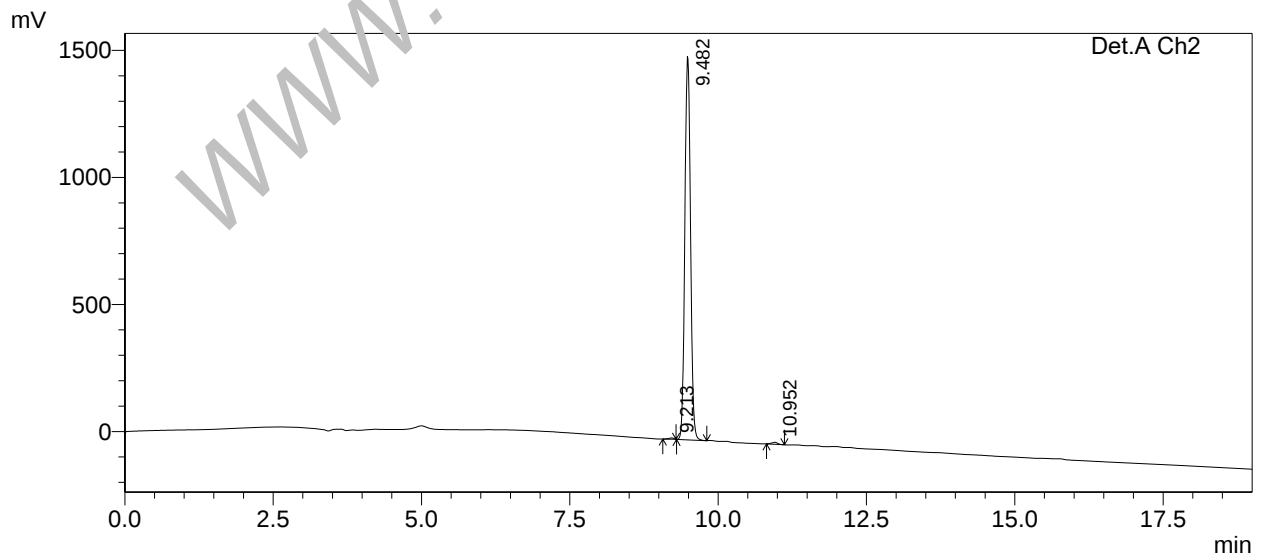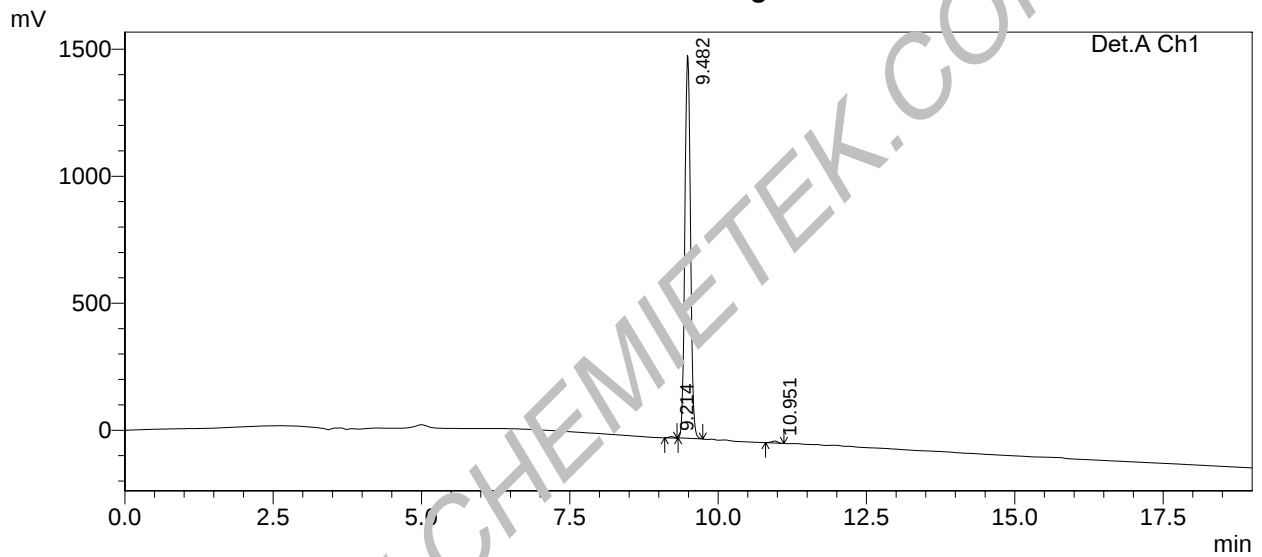

PeakTable

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %	Height %
1	9.214	31080	5321	0.307	0.350
2	9.482	10027777	1508253	99.111	99.131
3	10.951	58872	7903	0.582	0.519
Total		10117729	1521477	100.000	100.000

PeakTable

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %	Height %
1	9.213	32765	5412	0.323	0.356
2	9.482	10063665	1509118	99.129	99.136
3	10.952	55651	7734	0.548	0.508
Total		10152080	1522264	100.000	100.000

WWW.CHEMIETEK.COM