

CHEMIETEK HPLC-MS Report

File D:\DATA\A02\MONITOR\GSK-0924-7-06983-LCMSA009.D


Sample Name : GSK1070916-01
Acq. Operator : A02-Monitor
Spec. Reported : MS Integration
Acq. Method : D:\METHODS\2-POS-3MIN.M
Analysis Method : D:\METHODS\2-POS-3MIN.M

Tgt Mass(EZX) : 507.00
Location : P2-D-04
Inj : 1
Inj Volume : 2 ul




Sample Info : Easy-Access Method: '2-POS-3MIN' 507.00
Method Info : Column:Xbridge C18 (4.6x 50 mm, 3.5um)
Mobile phase: H2O(10 mmol NH4HCO3) (A) / ACN(B)
Elution program: Gradient from 10 to 95% of B in1.5min at 1.8ml/min
Temperature: 45 °C
Detection: UV (214 , 4 nm) and MS (ESI, Pos mode ,70 to 900 amu)


ADC1 A, ELSD

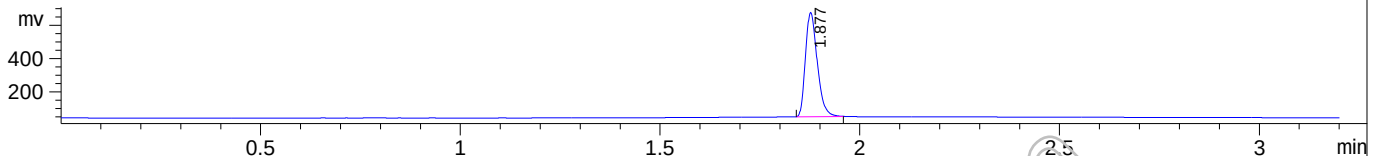


*DAD1 A, Sig=214,4 Ref=off

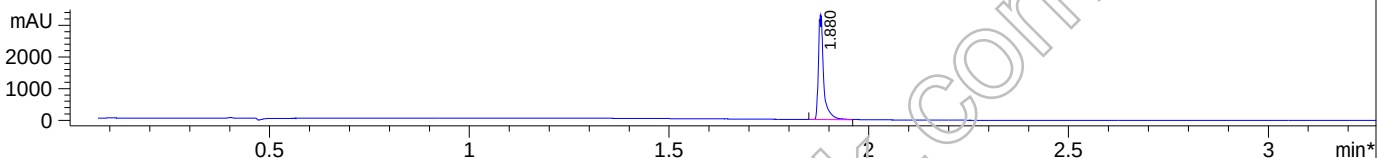


*DAD1 B, Sig=254,4 Ref=off

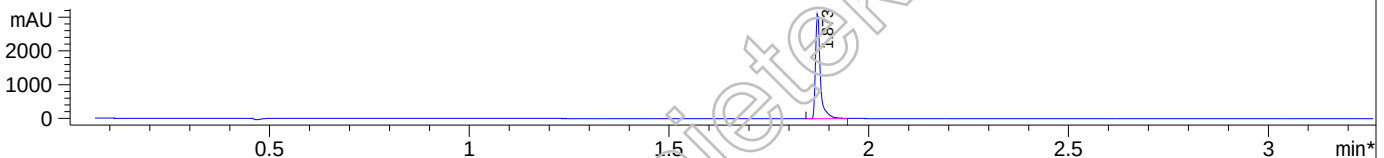

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 80

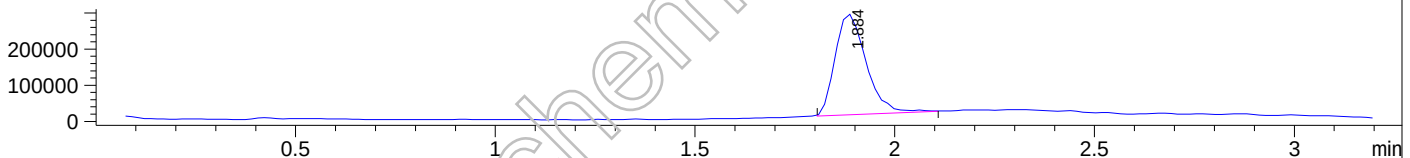

Ion 508, MSD1 508,Target Mass 507 +H Positive, EIC=507.7:508.7

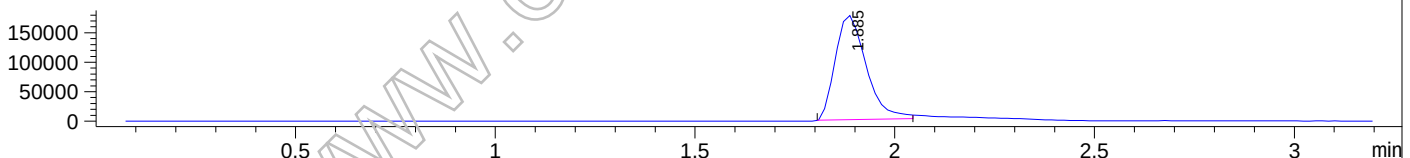

Integration Results for ADC1 A, ELSD


RetTim	Width	Area	Height	Area%
1.88	0.03	1299.46	627.65	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.88	0.02	3043.99	3099.18	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.87	0.02	2574.03	2826.05	100.00

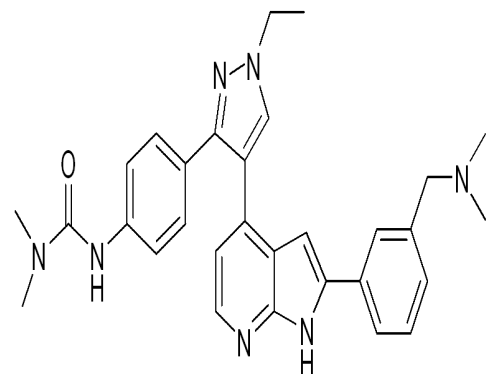

Ret. Time: 1.88 <<<< POSITIVE SPECTRA >>>>

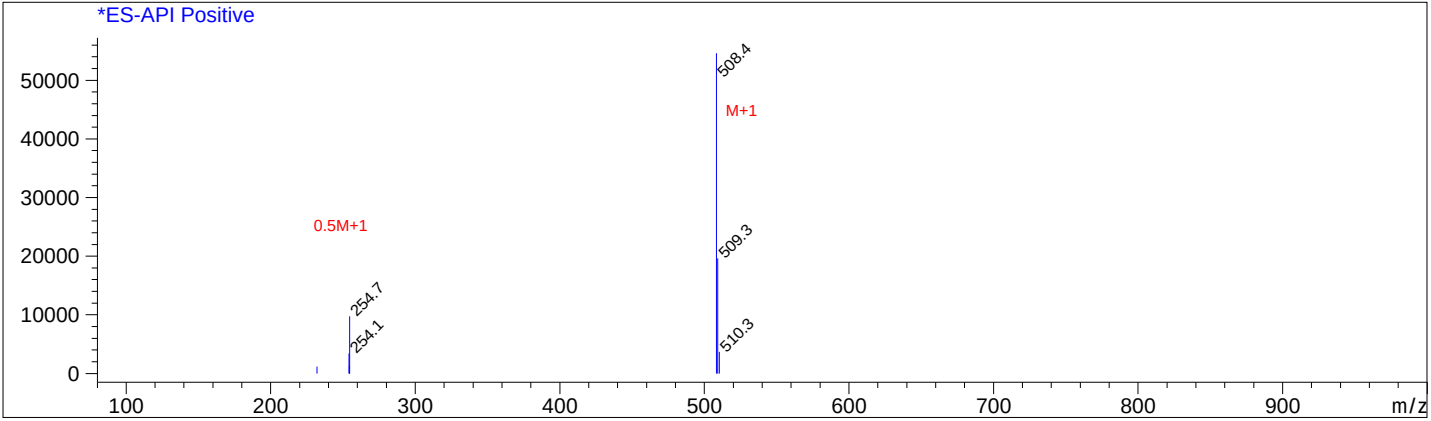

www.chemietek.com