


Sample Name : CT-GSK368-01
Acq. Operator : A02-Monitor
Spec. Reported : MS Integration
Acq. Method : D:\METHODS\HPLC-15MIN.M
Analysis Method : D:\METHODS\HPLC-15MIN.M
Sample Info : QC 15MIN Method: 'HPLC-15MIN.M'

Tgt Mass(EZX) :
Location : P1-D-08
Inj : 0
Inj Volume : 1 ul




For research information only. The test was performed
under R&D condition, Not for regulatory-filing purpose.

DAD1 A, Sig=214,4 Ref=off

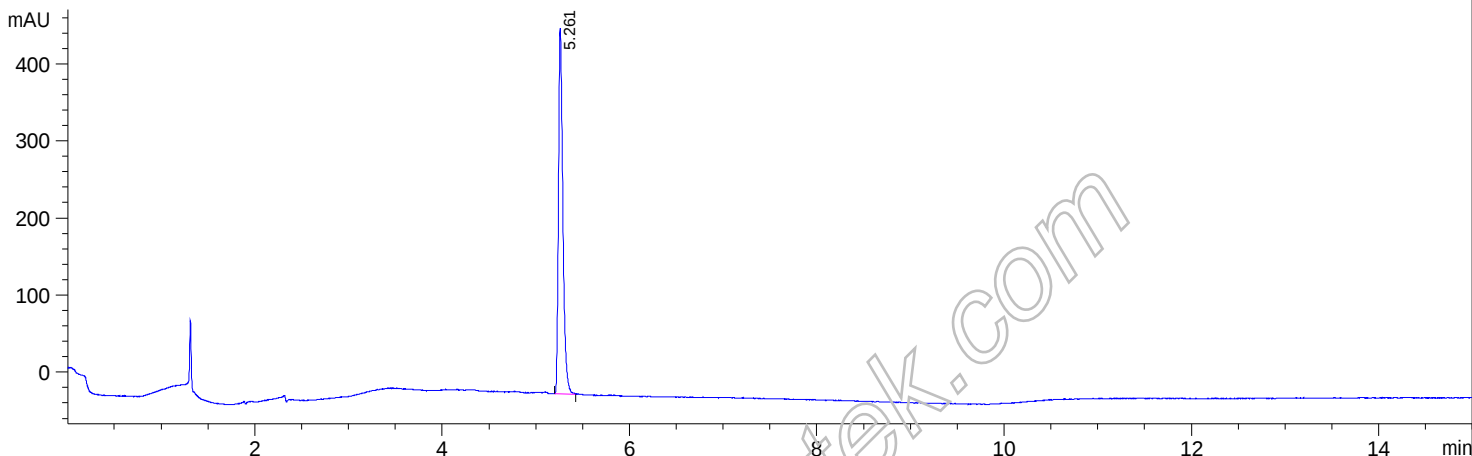

DAD1 B, Sig=254,4 Ref=off

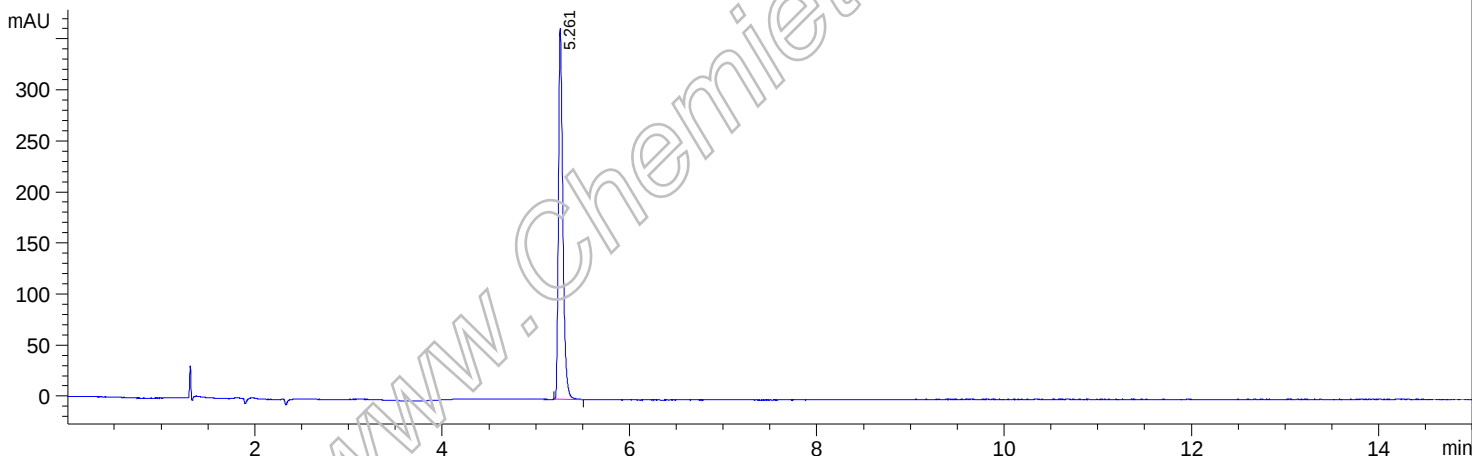

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.26	0.05	1533.16	474.57	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.26	0.05	1179.26	363.67	100.00

