

File D:\DATA\A52\MONITOR\CT-IACS13909-01-P-5963-LCMSA013.D

Sample Name : CT-IACS13909-01

Acq. Operator : A52-MONITOR

Spec. Reported : MS Integration

Acq. Method : D:\METHODS\QC-HPLC-15MIN.M

Analysis Method : D:\METHODS\QC-HPLC-15MIN.M


Sample Info : QC-15MIN Method: 'QC-15MIN' 376.00

Tgt Mass(EZX) : 376.00


Location : P2-F-01

Inj : 1


Inj Volume : 1.5 uL

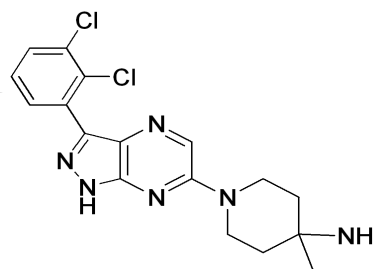


*ADC1 A, ELSD

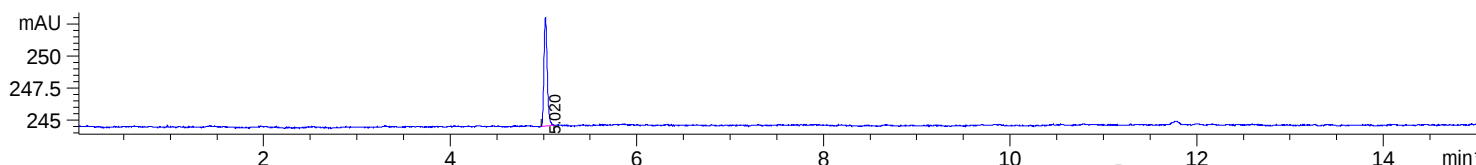


*DAD1 A, Sig=214,4 Ref=off

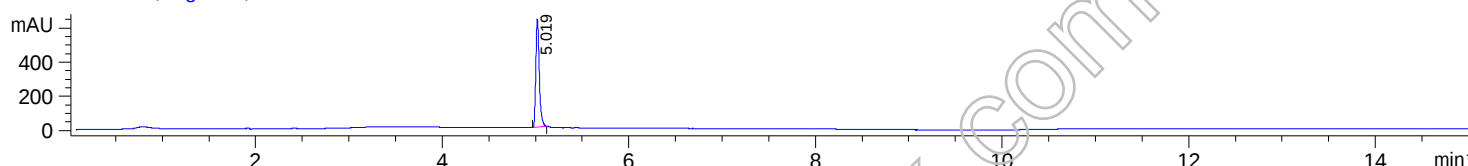


*DAD1 B, Sig=254,4 Ref=off

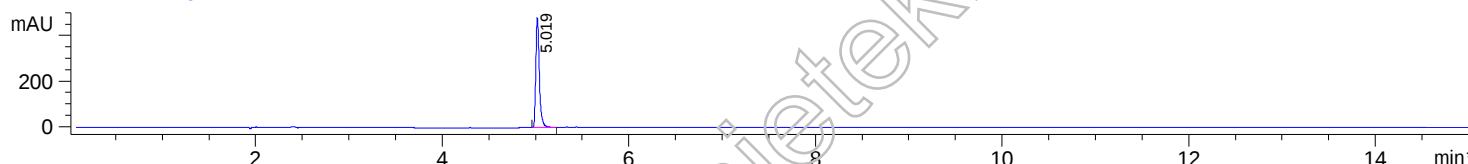

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

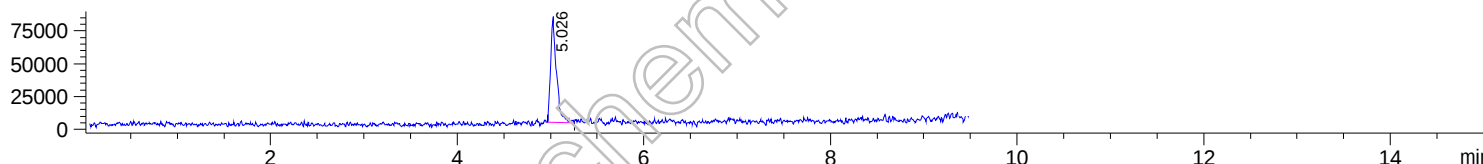

Ion 377, MSD1 377, Target Mass 376 +H Positive EIC=376.7:377.7

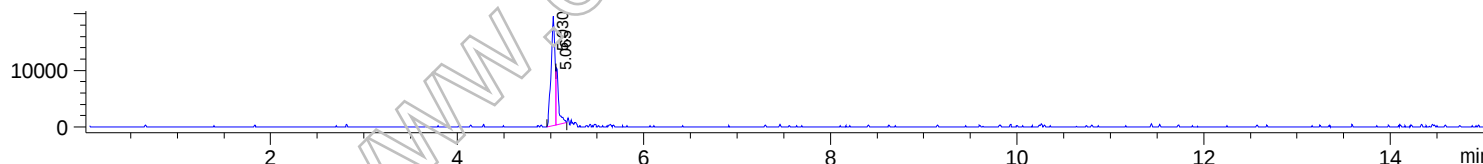

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
5.02	0.04	20.61	8.47	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.02	0.04	1617.96	631.22	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.02	0.04	1262.92	480.73	100.00

Ret. Time: 5.03

<<<< POSITIVE SPECTRA >>>>

