
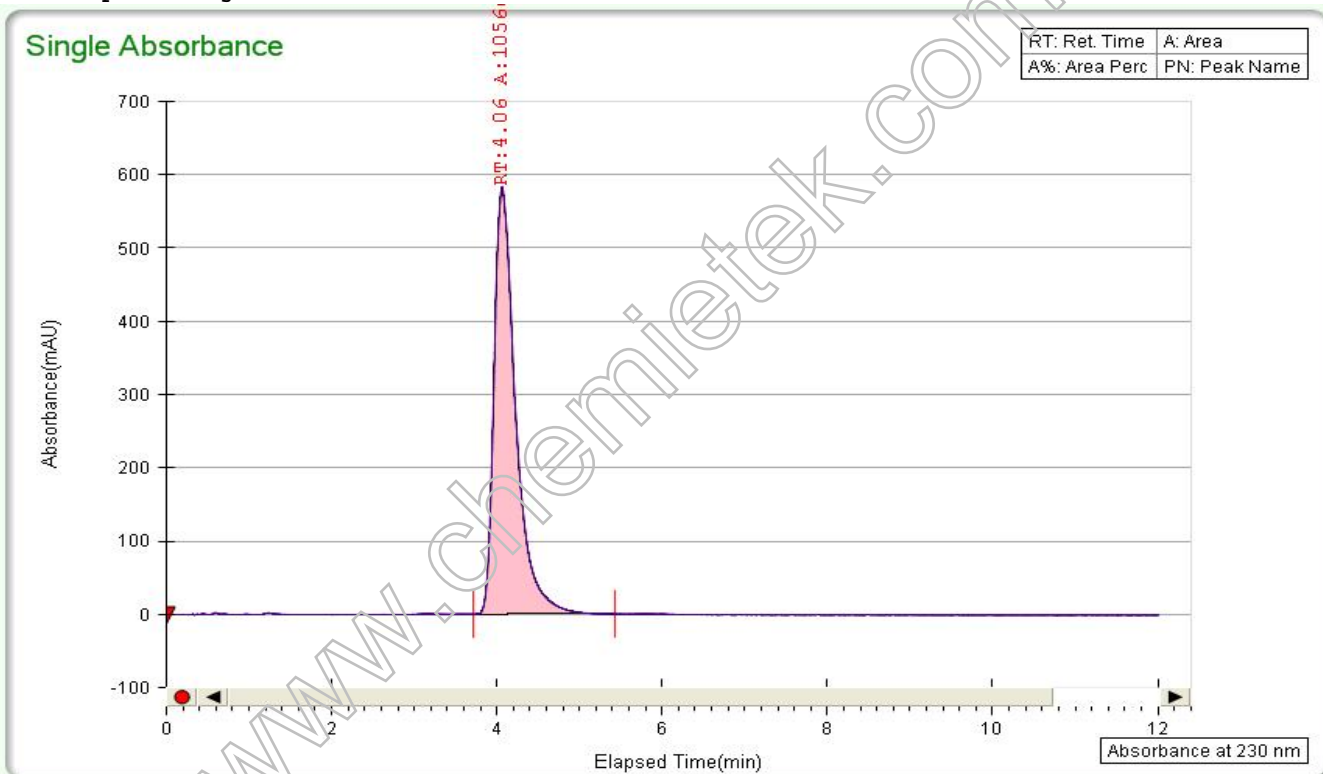


CHEMIETEK Chiral HPLC Report

Injection Info
Injection Date Time Stamp Default
Injection Volume 3
Co-Solvent MeOH(0.2%Methanol Ammonia)
Column
Sample IPI-549 Chemietek Lot 2
Sample Well P1: 5D
Column Temperature 40
CO2 Flow Rate 2.8
Co-Solvent Flow Rate 1.2
Co-Solvent % 30
Total Flow 4
Front Pressure 156
Back Pressure 120
Pressure Drop 36
PDA Start Wavelength 214
PDA Stop Wavelength 359

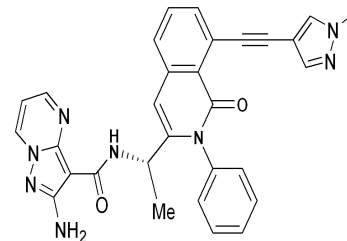

Peak Info

Number	RT (min)	Area %	Area	Height
1	4.06	100	10566.6861	583.5297