





Sample Name : IPI549 Lot 04
Tgt Mass (EZ) : 528
Acq. Operator : ADMIN
Spec. Reported : MS Integration
Acq. Method : D:\METHODS\Documents\1-CHEMIELAB-HPLC-15MIN.M
Analysis Method : D:\METHODS\1-CHEMIELAB-HPLC-15MIN.M
Sample Info : CHEMIELAB HPLC Method: '1-CHEMIELAB-HPLC-15MIN.M'
Method Info : Default Method


*DAD1 A, Sig=214,4 Ref=off

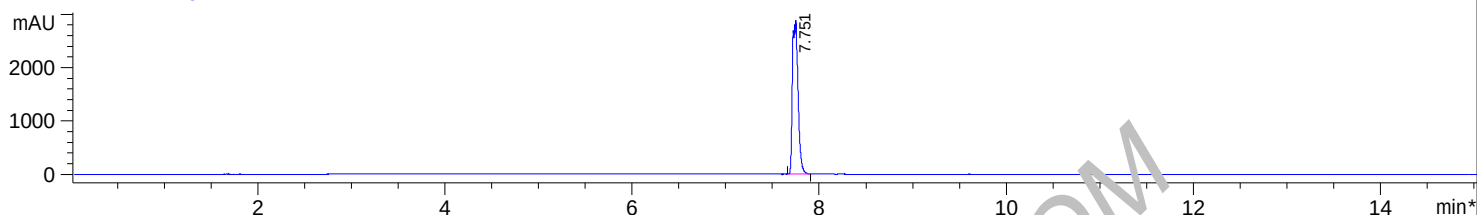


*DAD1 B, Sig=254,4 Ref=off

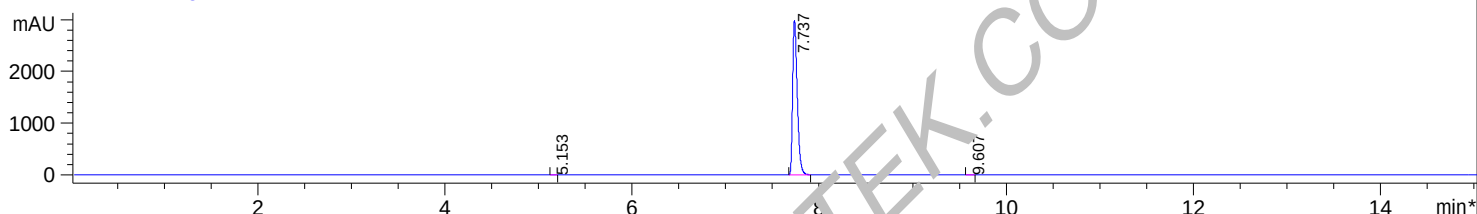

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

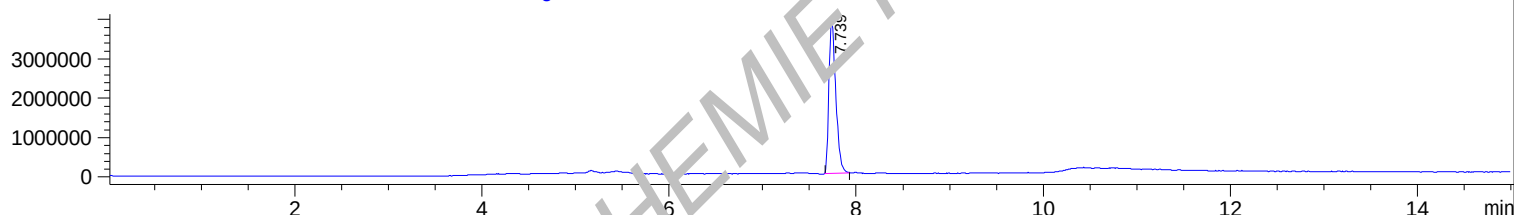

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7,1.7

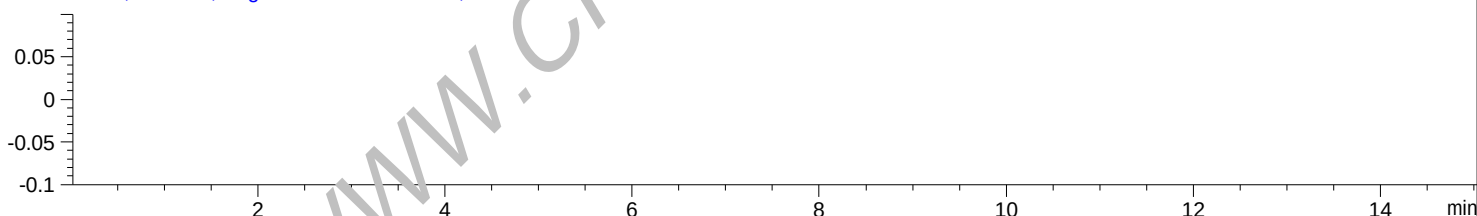


Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.75	0.05	11931.41	2834.81	100.00


Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.15	0.02	5.60	2.79	0.05
7.74	0.04	10259.45	2987.21	99.82
9.61	0.04	13.18	5.07	0.13

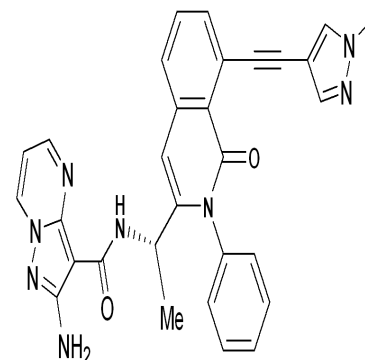

Ret. Time: 7.74

<<<< POSITIVE SPECTRA >>>>

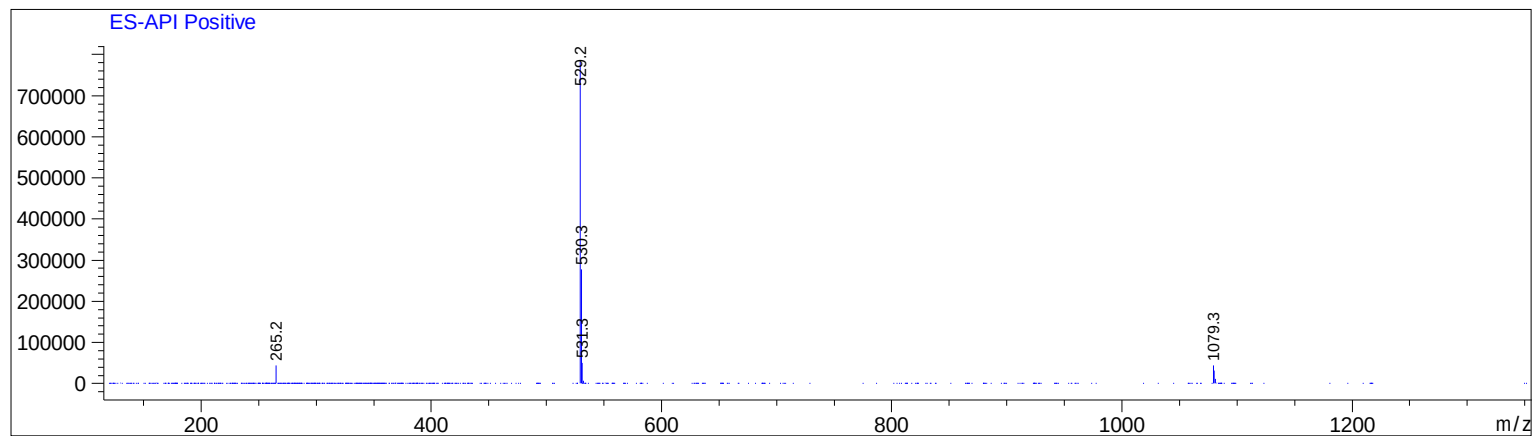

WWW.CHEMIETEK.COM