





=====

Acq. Operator : Admin
Acq. Instrument : HPLCAB
Location : P1-D-02
Inj Volume : 2.0 µl
Method : D:\METHODS\2-CHEMIETEK-HPLC-15MIN.M
Last changed : Default by Admin
(modified after loading)

Method Info : Mobile Phase: Default
Gradient: Default

Sample Info : 2-CHEMIELAB-HPLC-15MIN.M

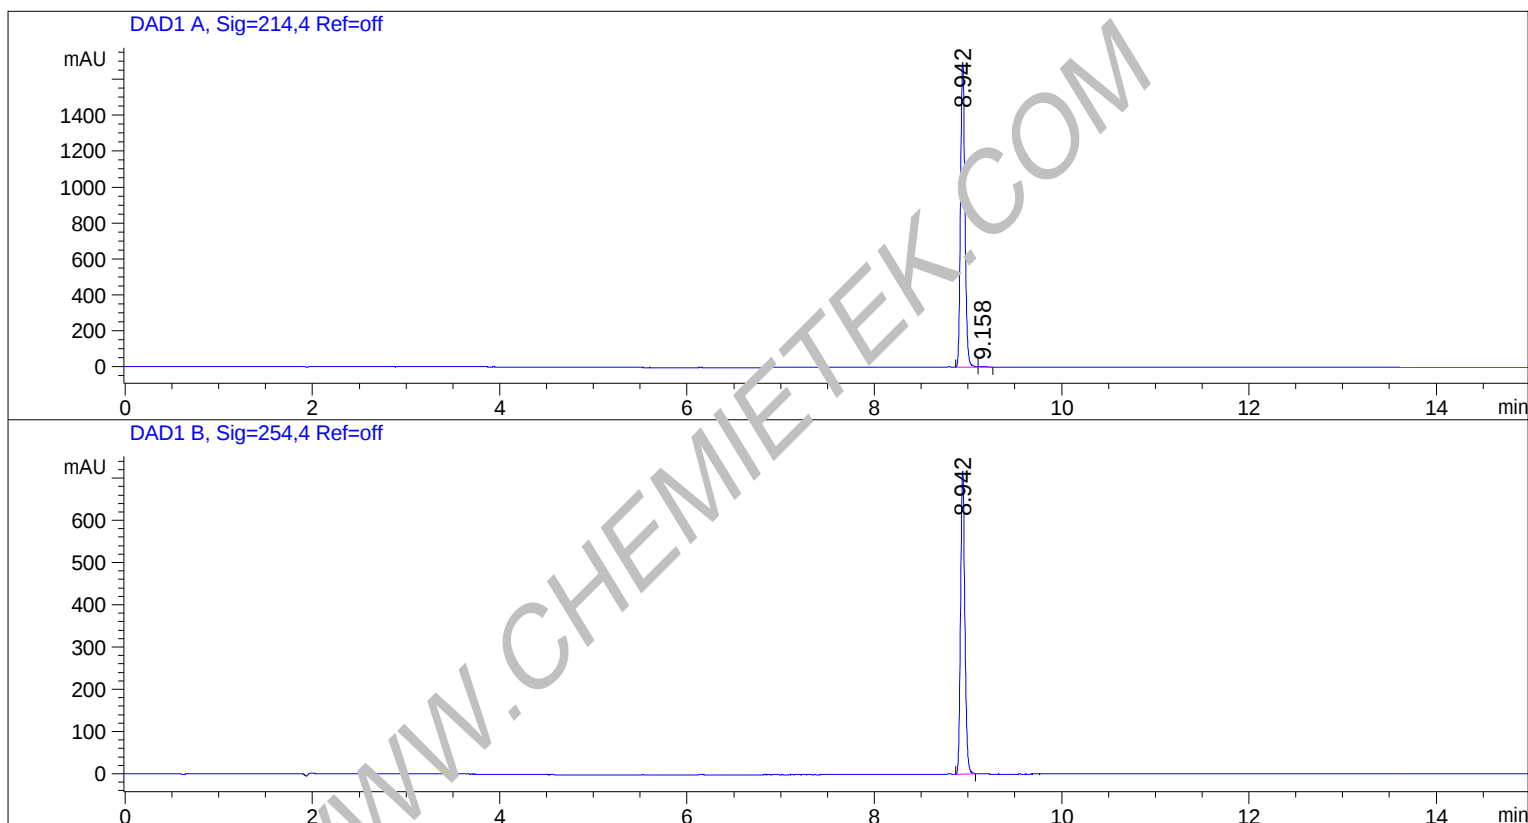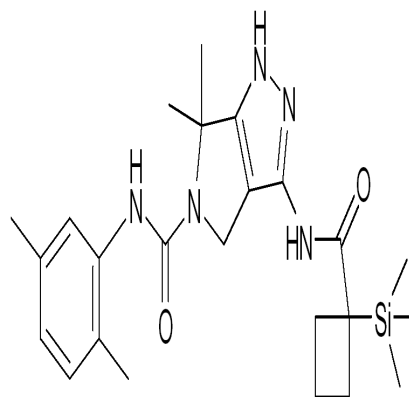

=====

Area Percent Report

=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.942	BB	0.0531	5694.87939	1698.68140	99.6871
2	9.158	BB	0.0693	17.87698	3.91064	0.3129

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
----	-----	----	-----	-----	-----	-----
Totals :				5712.75638	1702.59204	

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
----	-----	----	-----	-----	-----	-----
1	8.942	BB	0.0501	2344.56152	718.58655	100.0000
Totals :				2344.56152	718.58655	

=====
*** End of Report ***