
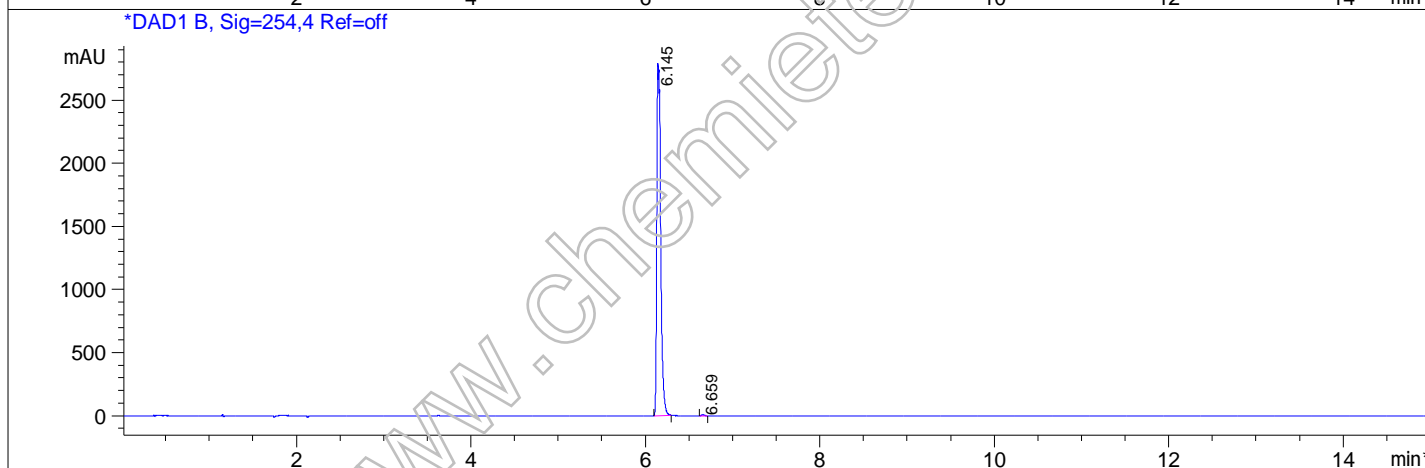


File ..\MONITOR\CTK-000049-037-A-145217-LCMSA033.DTgt Mass(EZX):
 Seq. Line: 0
 Location: P2-A-04
 Sample Name : LOXO-195 CTK Lot -01
 Acq. Operator : A02-MONITOR
 Spec. Reported : MS Integration
 Acq. Method : D:\METHODS\2-HPLC-CHEMIELABS.M
 Analysis Method : D:\METHODS\2-HPLC-CHEMIELABS.M
 Sample Info : Easy-Access Method: '2-HPLC-CHEMIELABS'
 Method Info : Mobile Phase: A: water(10mMNH4HCO3) B: ACN
 Gradient
 Time 0 7.5 15
 B % 5 95 95
 Flow Rate: 1.0mL/min
 Oven temperature: 50C

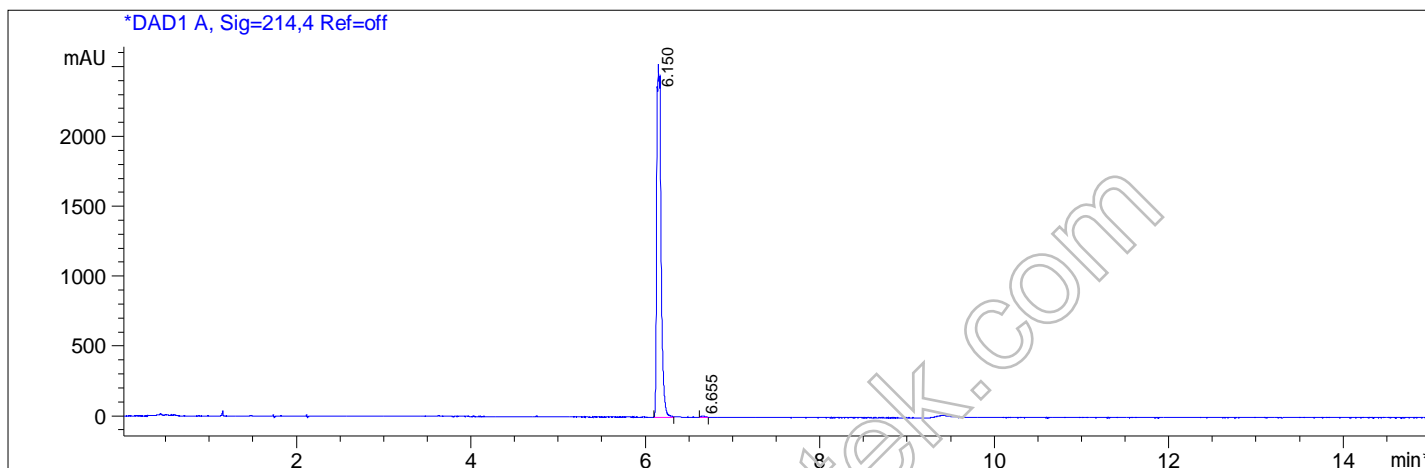

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
6.15	0.04	8724.84	2523.11	99.72
6.66	0.04	24.67	10.17	0.28

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.14	0.04	8679.45	2781.22	99.74
6.66	0.03	22.44	9.23	0.26

