



CHEMIETEK Chiral HPLC Report

Injection Info

Injection Volume 5
Co-Solvent
Column
Sample M2698-01-CHEMIETEK
Sample Well P1: 5D
Column Temperature 40.1
C02 Flow Rate 3.2
Co-Solvent Flow Rate 0.8
Co-Solvent % 20
Total Flow 4
Front Pressure 152
Back Pressure 122
Pressure Drop 30
PDA Start Wavelength 214
PDA Stop Wavelength 359

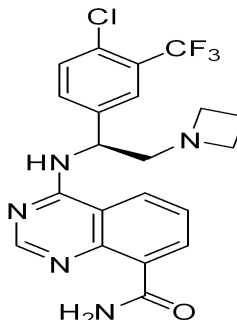

Single Absorbance

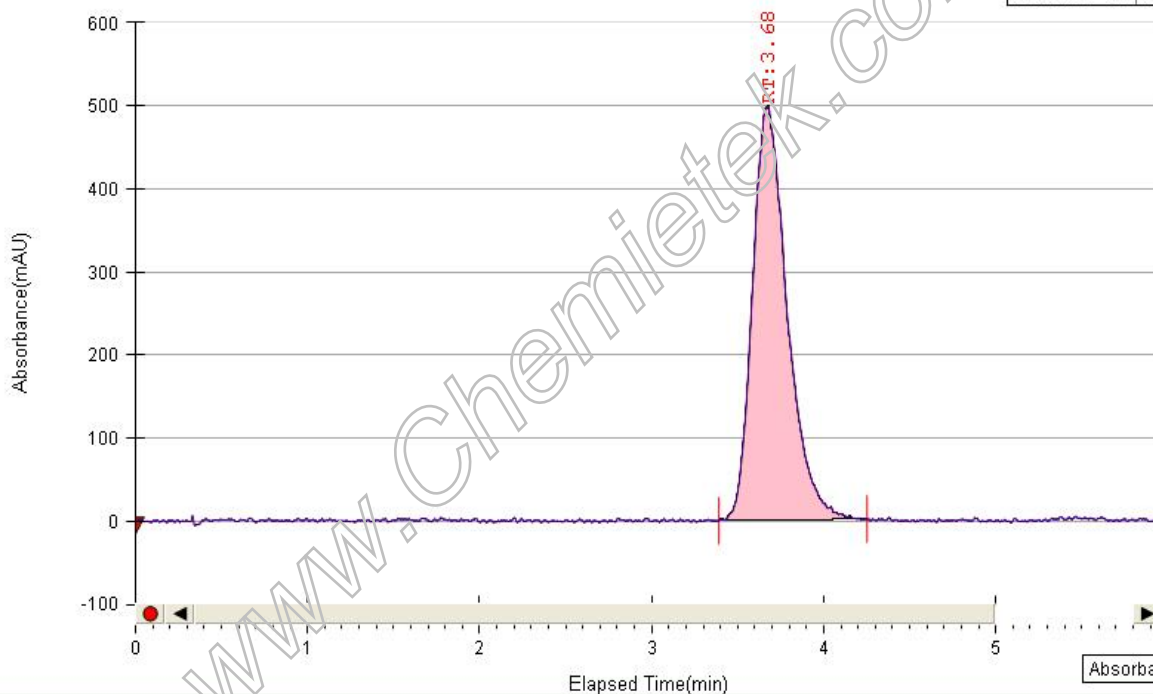

RT: Ret. Time	A: Area
A%: Area Perc	PN: Peak Name

Peak Info

Number	RT (min)	Area %	Area	Height
1	3.68	100	6981.0734	499.4674