



Sample Name : CT-MG265 Lot 02

Location : P2-F-09

Acq. Operator : T245-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 0.5 ul

Acq. Method : D:\METHODS\QC-HPLC-3MIN.M

Analysis Method : D:\METHODS\QC-HPLC-3MIN.M

Sample Info : Easy-Access Method: '1-POS-3MIN'

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)






Gradient: 5% increase to 95%B within 1.3 min, 95%B for 1.7

Flow Rate: 2.0ml/min

Column:Sunfire C18,4.6*50mm,3.5um

Column Temperature: 45 C

Detection:UV(214,4nm) and MS(ESI,Pos mode,110 to 1000 amu)

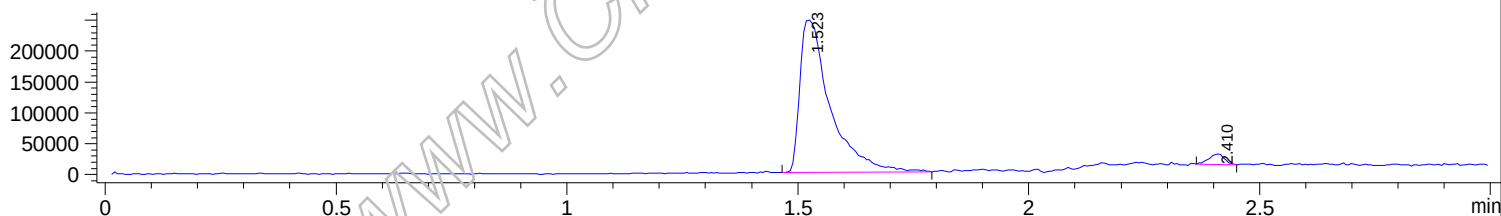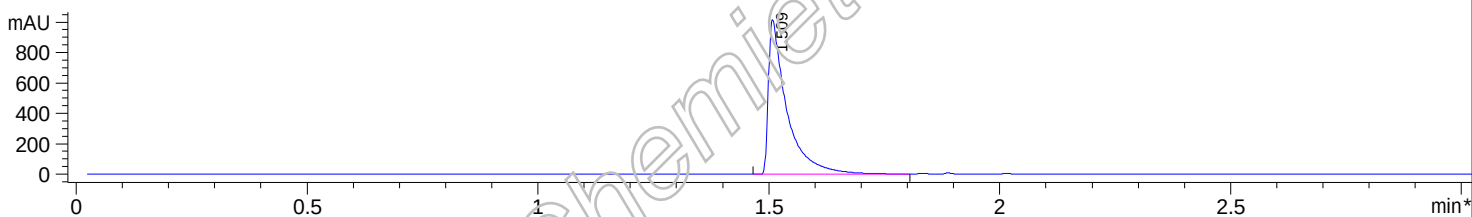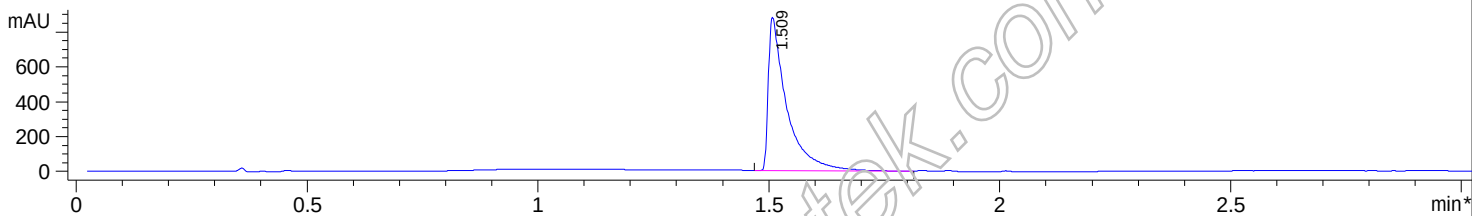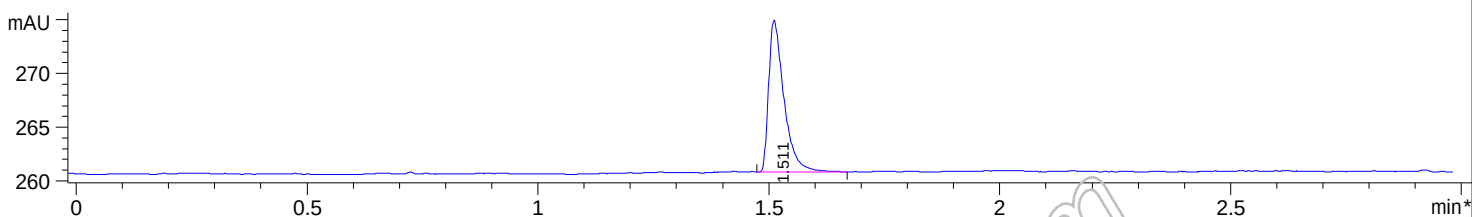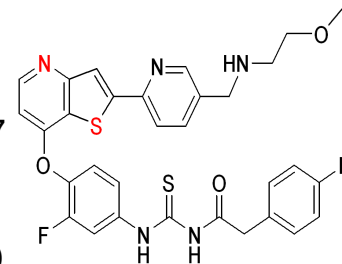

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.51	0.03	32.60	14.18	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.51	0.04	2428.20	878.91	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.51	0.04	2788.54	1015.59	100.00

Ret. Time: 1.52

<<<< POSITIVE SPECTRA >>>>

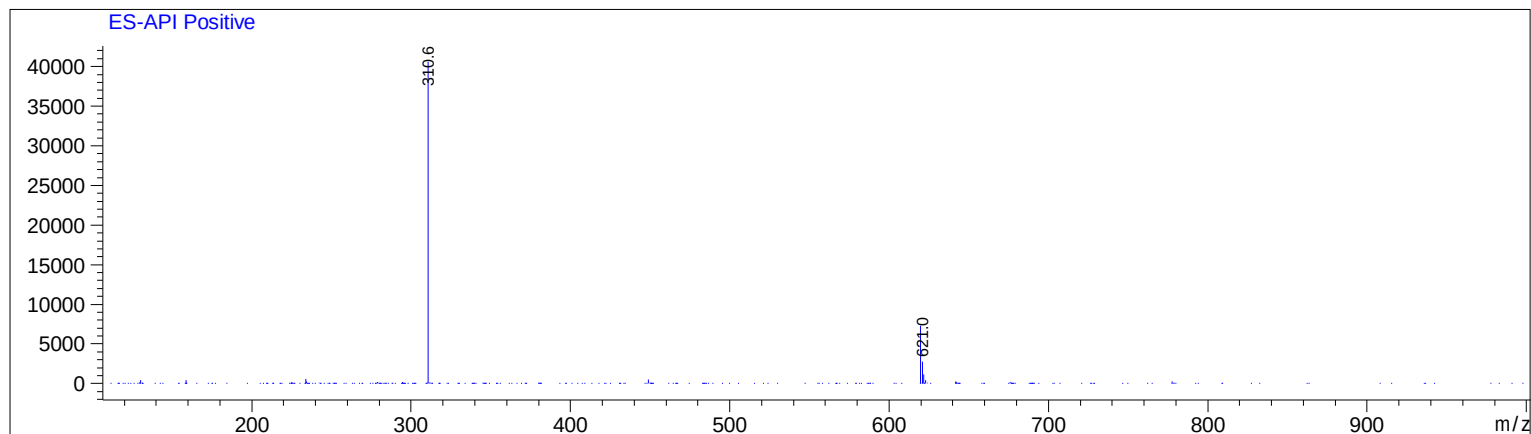

Ret. Time: 2.41

