

File D:\DATA\A02\RS-MK5108-00888-HPLCA004.D

Sample Name : MK5108 02

Acq. Operator : HPLCA004

Spec. Reported : MS Integration

Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Analysis Method : C:\CHEM32\1\METHODS\2-HPLC-15MIN.M

Sample Info :

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B

Flow Rate: 1.2 ml/min

Column: Eclipse XDB-C18,4.6*150mm,5um




Oven Temperature: 40 C

Tgt Mass(EZX) :

Location : P2-B-07


Inj : 0

Inj Volume : 7 u1

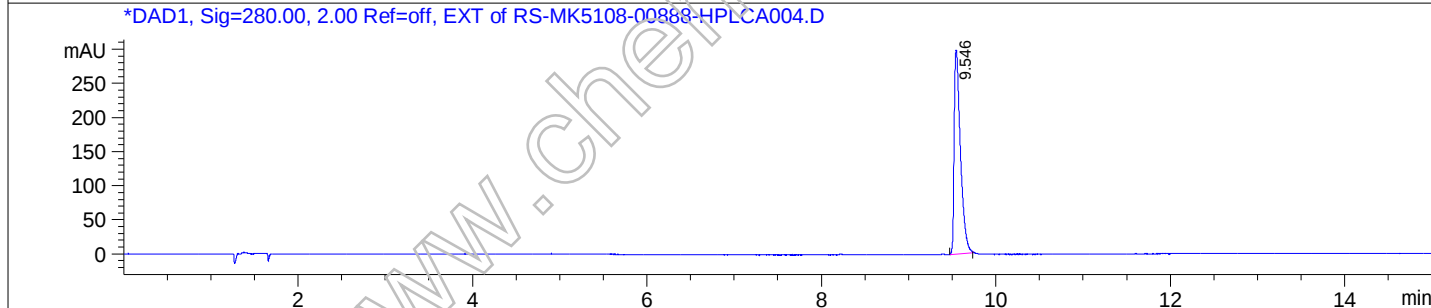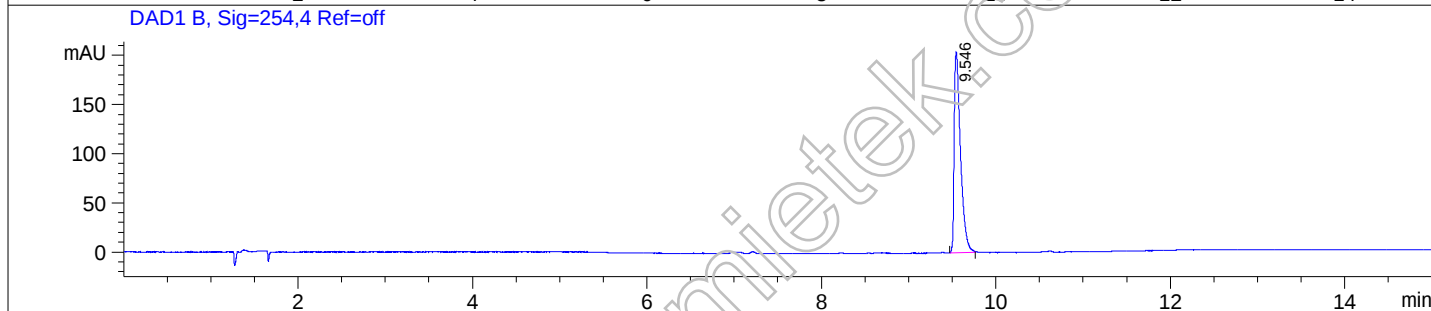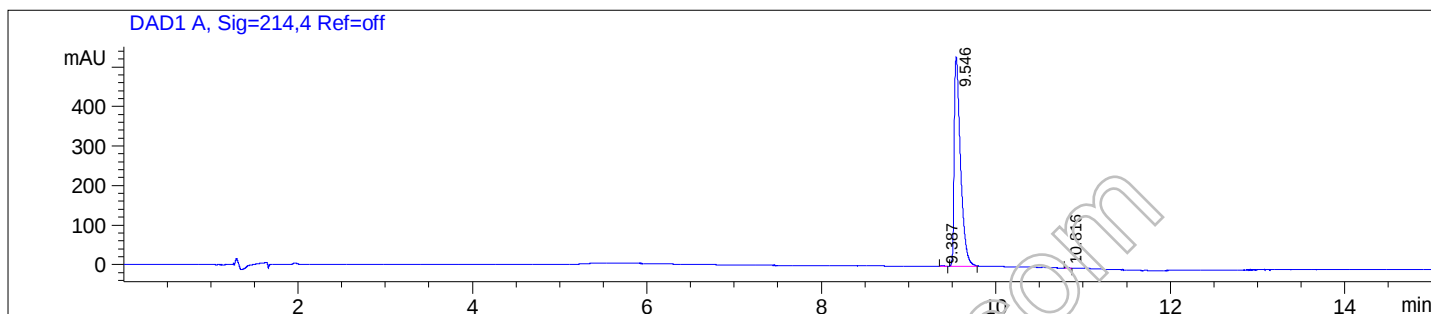

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
9.39	0.03	6.52	2.62	0.24
9.55	0.07	2671.35	529.37	99.58
10.82	0.03	4.74	2.02	0.18

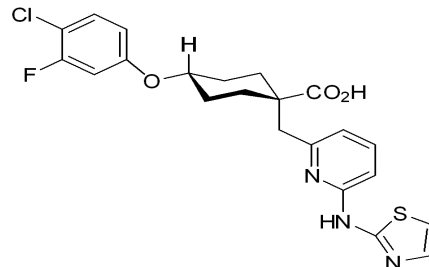

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
9.55	0.07	1025.30	204.14	100.00

Integration Results for DAD1, Sig=280.00, 2.00 Ref=off, EXT

RetTim	Width	Area	Height	Area%
9.55	0.07	1486.97	299.18	100.00