
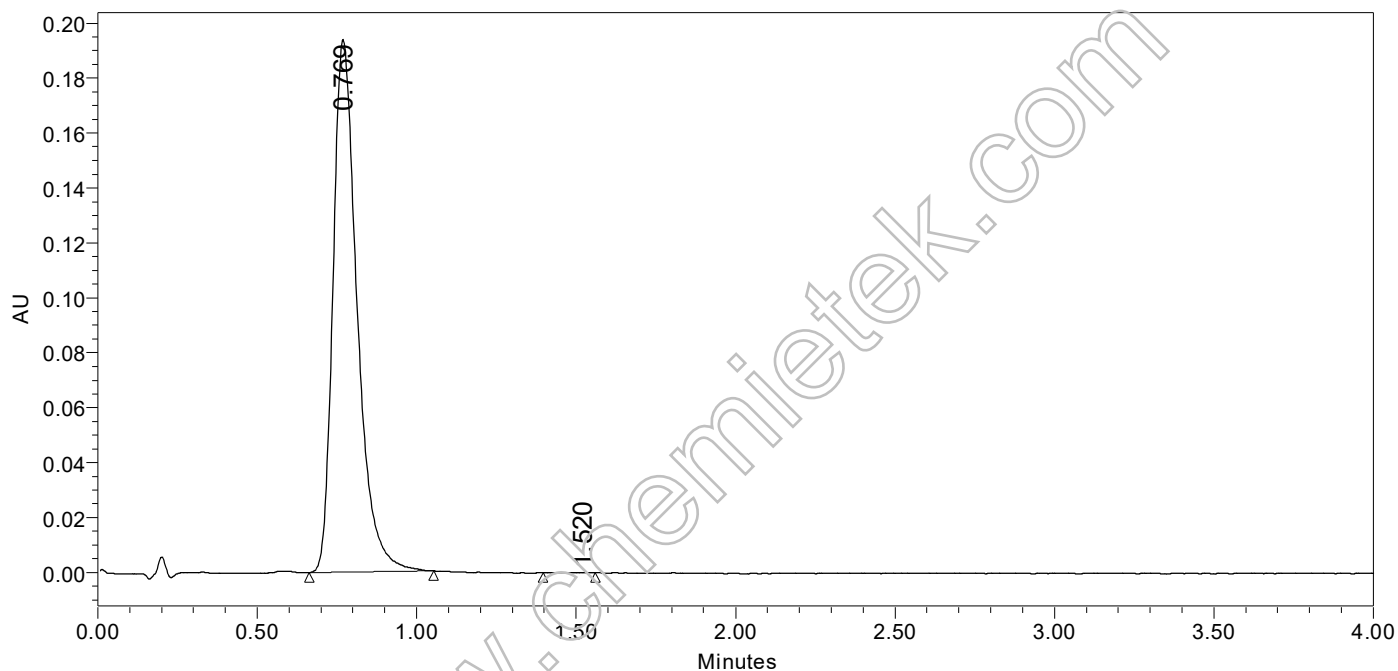


SAMPLE INFORMATION

Sample ID: Admin
 Compound ID: CT-PF0710 Lot 02
 Acq Method : IG_IPA_IPAm_40_4_35

Channel Name: 220.0nm

User Name: Admin
 Instrument: Waters UPCC with ODA

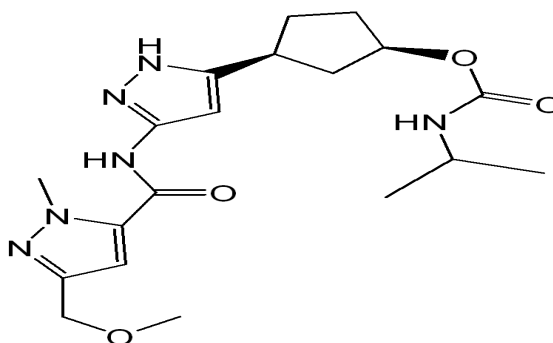

	RT	Area	% Area*	Height
1	0.769	1016961	99.89	193905
2	1.520	1109	0.11	196