



File D:\DATA\C66\MONITOR\RMC_6236-02-64598-LCMSA027.D


Sample Name : RMC-6236 Lot 02
Acq. Operator : ADMIN
Spec. Reported : MS Integration
Acq. Method : D:\METHODS\1-CHEMIELAB-HPLC-3MIN.M
Analysis Method : D:\METHODS\1-CHEMIELAB-HPLC-3MIN.M
Sample Info : CHEMIELAB HPLC Method: '1-CHEMIELAB-HPLC-3MIN.M'
Method Info : Default Method

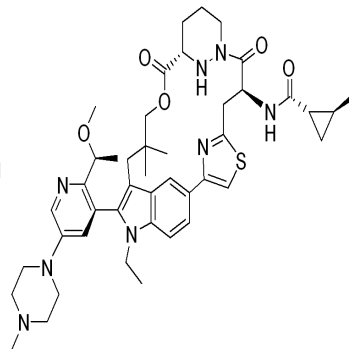


*DAD1 A, Sig=214,4 Ref=off

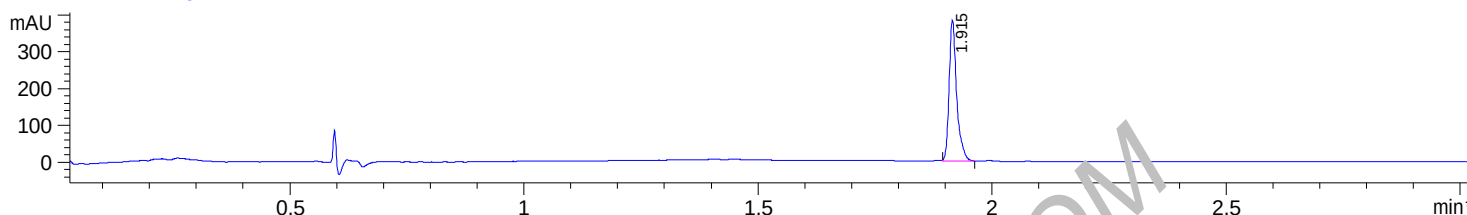


*DAD1 B, Sig=254,4 Ref=off

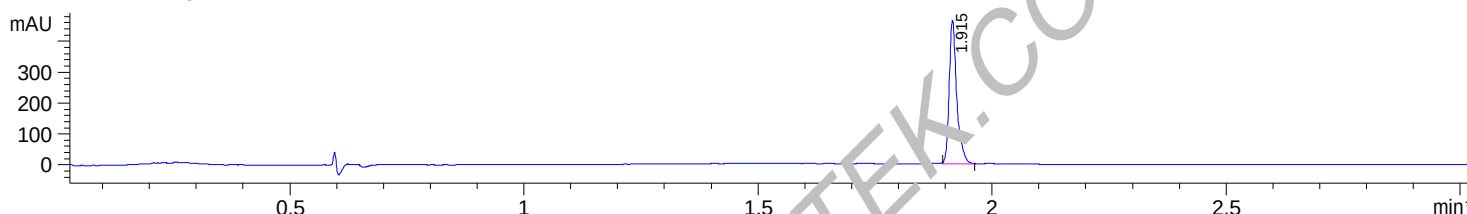

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

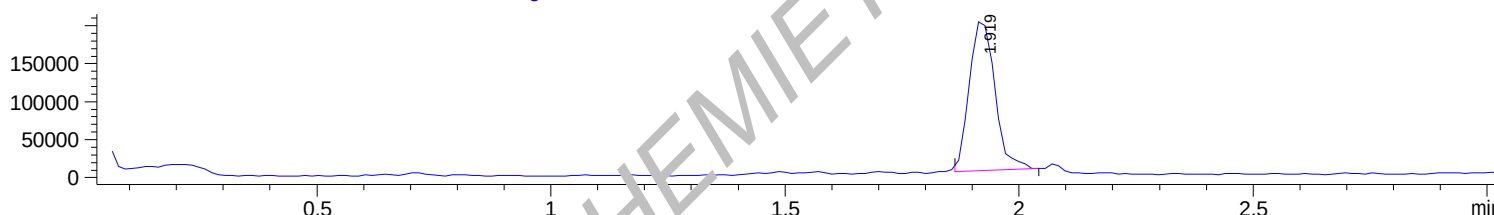

Ion 811, MSD1 811, Target Mass 810 +H Positive, C10 810.7-811.7

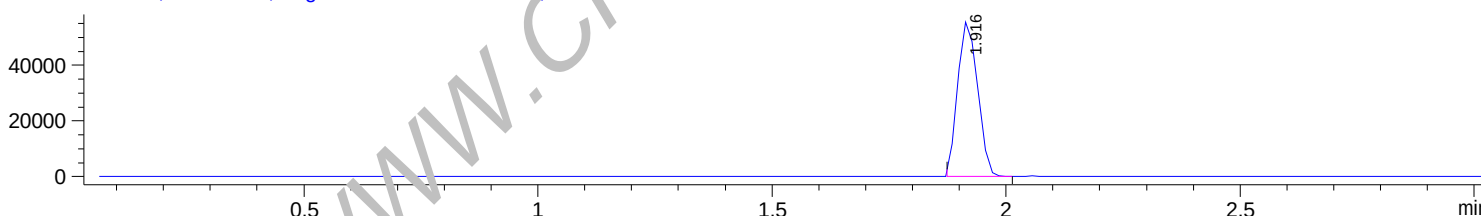

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.92	0.02	427.50	382.18	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.92	0.02	518.90	463.16	100.00

Ret. Time: 1.92

<<<< POSITIVE SPECTRA >>>>

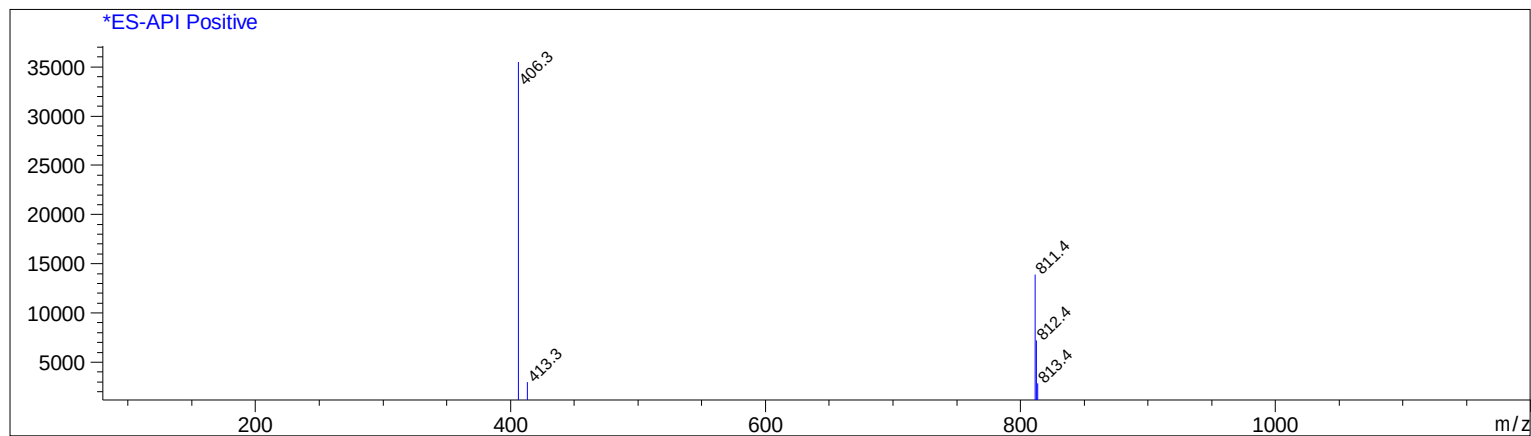

WWW.CHEMIETEK.COM