

Sample Name: RX-5902 Chemietek Lot 01

Acq. Operator : CTK

Acq. Instrument : HPLCA004


Location : P1-D-01



Method : D:\METHODS\1-HPLC-15MIN-2.M

(modified after loading)
Method Info : Mobile Phase: A: water(0.05%TFA) B: ACN(0.05%TFA)
Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B
Flow Rate: 1.2 ml/min
Column: Eclipse XDB-C18,4.6*150mm,5um
Oven Temperature: 40 C

Sample Info : Easy-Access Method: '1-HPLC-15MIN-2'

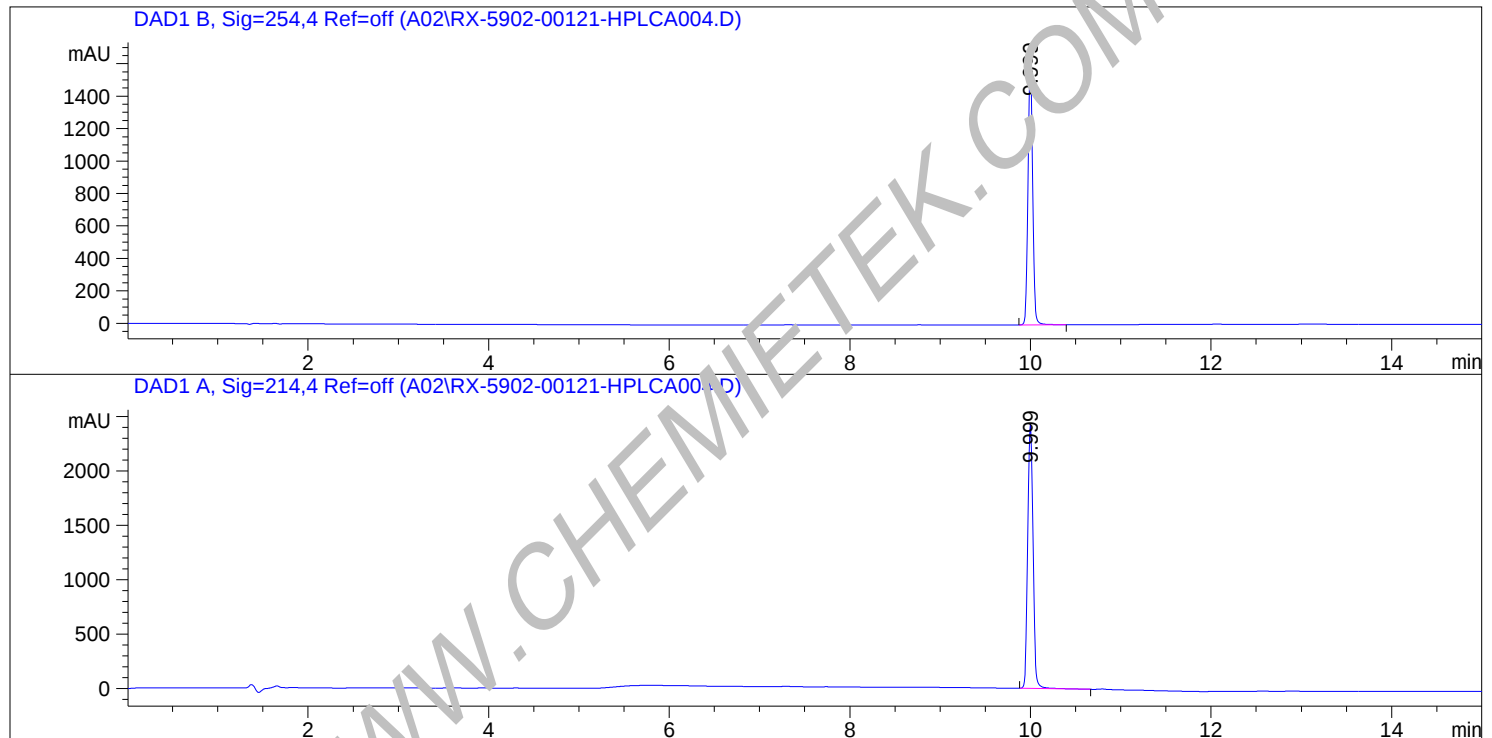


Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	9.999	BB	0.0552	5849.59424	1658.28784	100.0000

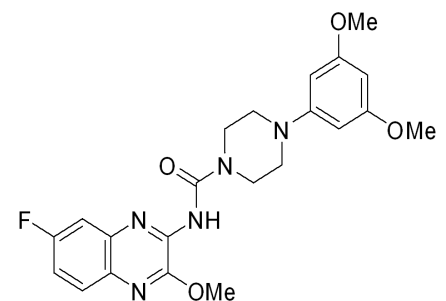




Totals : 5849.59424 1658.28784

Signal 2: DAD1 A, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	9.999	BB	0.0663	1.00984e4	2438.73340	100.0000

Totals : 1.00984e4 2438.73340

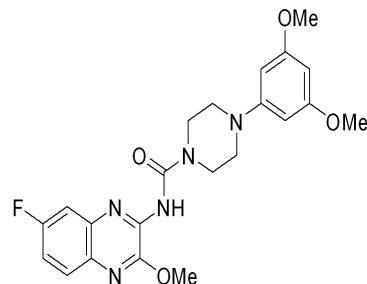

*** End of Report ***

WWW.CHEMIETEK.COM