



Acq. Operator : Admin
Acq. Instrument : HPLCA004

Location : P1-C-01



Inj Volume : 2.0 µl

Method : C:\CHEM32\1\METHODS\2-HPLC-15MIN.M

(modified after loading)

Method Info : Mobile Phase: A: water(0.05%TFA) B: ACN(0.05%TFA)
Gradient: 5% increase to 95%B within 8 min, 95%B for 7 min.
Flow Rate: 1.0ml/min
Column:
Column Temperature:40 C

Sample Info :

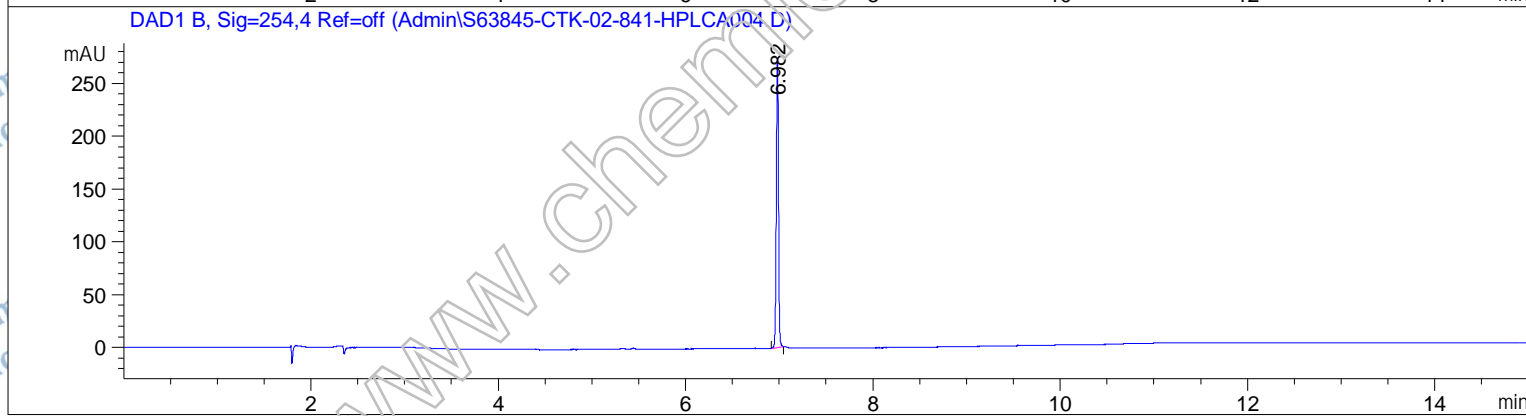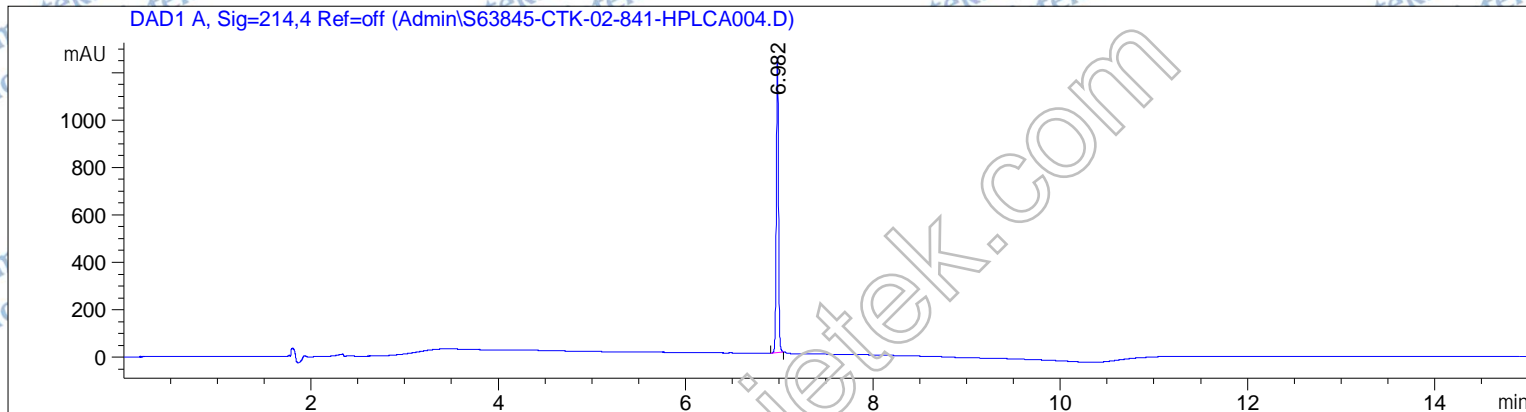


Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=214, 4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.982	BB	0.0248	2006.80688	1244.96790	100.00

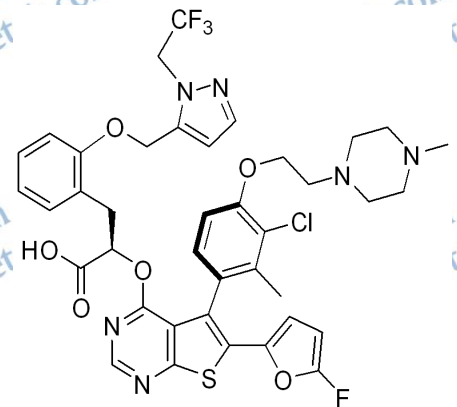

Totals : 2006.80688 1244.96790

Signal 2: DAD1 B, Sig=254, 4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.982	BB	0.0247	440.20041	273.93286	100.00

Totals : 440.20041 273.93286

=====
*** End of Report ***