
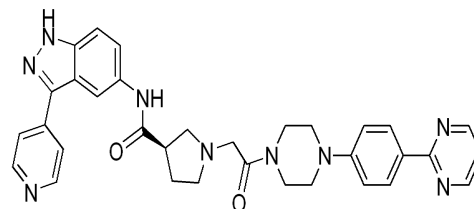
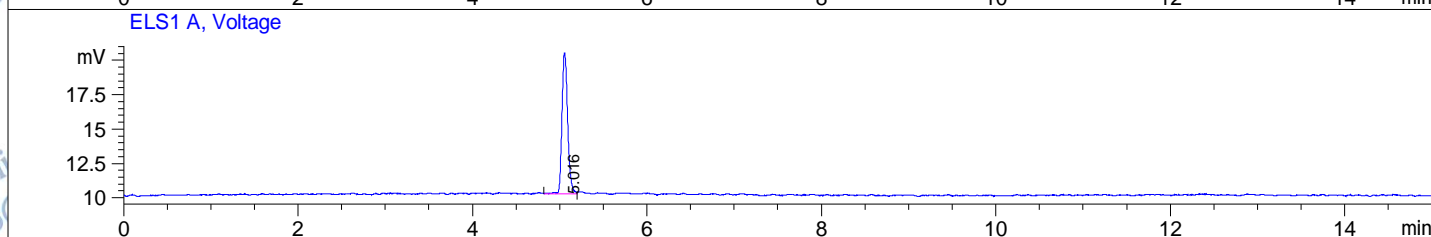
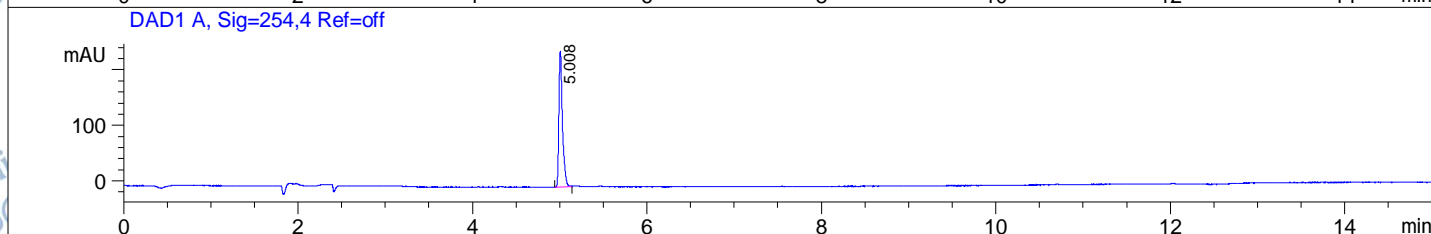


File ..06\MONITOR\SCH-772984-03-1-HG-36722-LCMSA042.D Tgt Mass (EZX):
 Seq. Line : 0
 Location : P2-A-09
 Sample Name : SCH-772984-03-Chemie
 Acq. Operator : 06monitor
 Inj : 1
 Spec. Reported : MS Integration
 Inj Volume : 5 ul
 Acq. Method : C:\CHEM32\1\METHODS\HPLC-A.M
 Analysis Method : C:\CHEM32\1\METHODS\HPLC-A.M
 Sample Info : Easy-Access Method: 'HPLC-A.M'
 Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;
 Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;
 Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;
 Flow Rate: 1.0 mL/min;
 Column Temperature: 40 °C

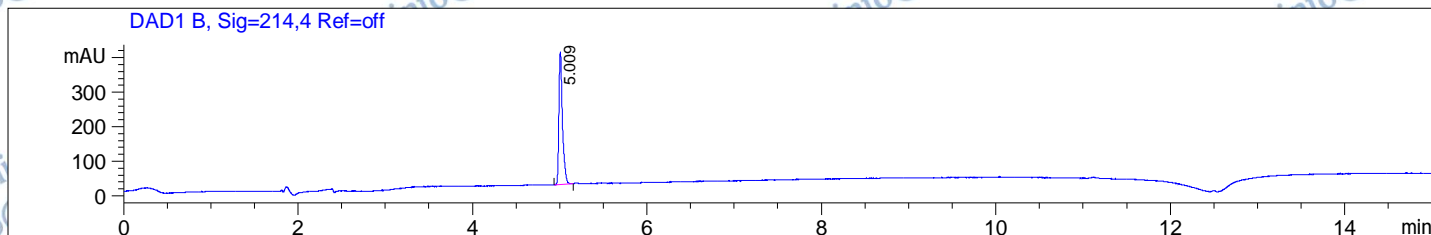

Integration Results for DAD1 B, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
5.01	0.05	1082.75	376.68	100.00

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.01	0.04	685.82	242.15	100.00

Integration Results for ELS1 A, Voltage

RetTim	Width	Area	Height	Area%
5.02	0.07	47.18	10.27	100.00

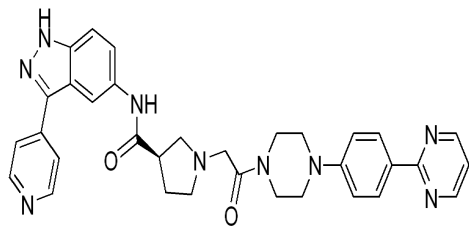

Ret. Time: 5.01

