

File D:\DATA\A2\MONITOR\CTK-0022485-083-02716-LCMSA013.D

Tgt Mass(EZX) : 691.00

Sample Name : CT-SCH353 01 Location : V1-C-12

Acq. Operator : A2-AdMIN

Spec. Reported : MS Integration Inj Volume : 2 ul

Acq. Method : D:\METHODS\QC-HPLC-15MIN.M

Analysis Method : D:\METHODS\QC-HPLC-15MIN.M

Sample Info : QC 15min Method: 'QC-HPLC-15MIN.M'

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.


Flow Rate: 1.0ml/min

Column:Sunfire C18,4.6\*150mm,3.5um


Column Temperature: 45 C



DAD1 A, Sig=214,4 Ref=off

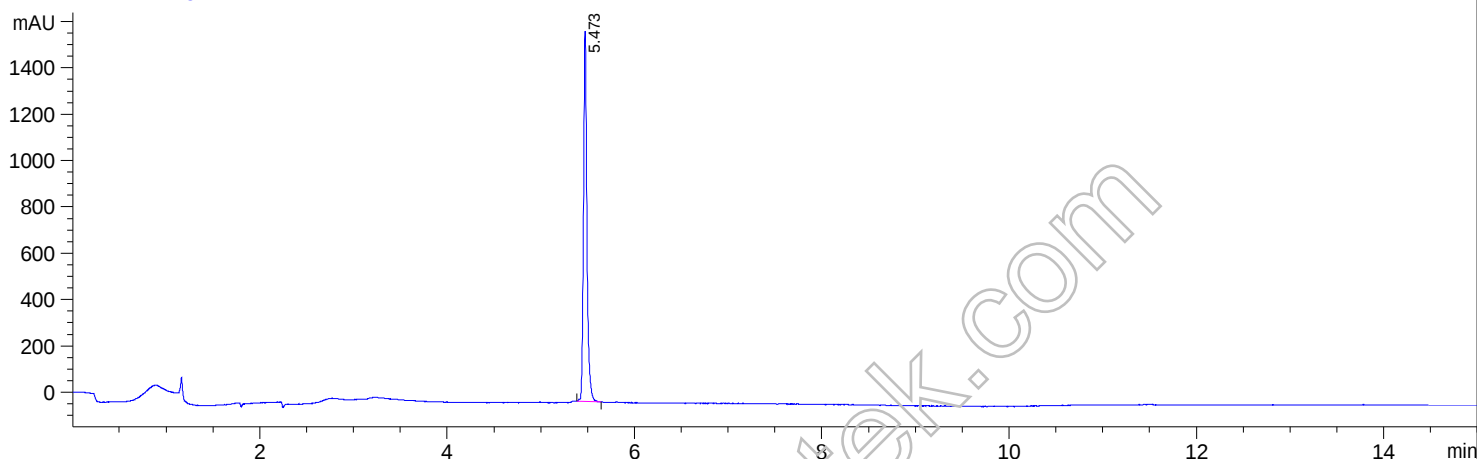

DAD1 B, Sig=254,4 Ref=off

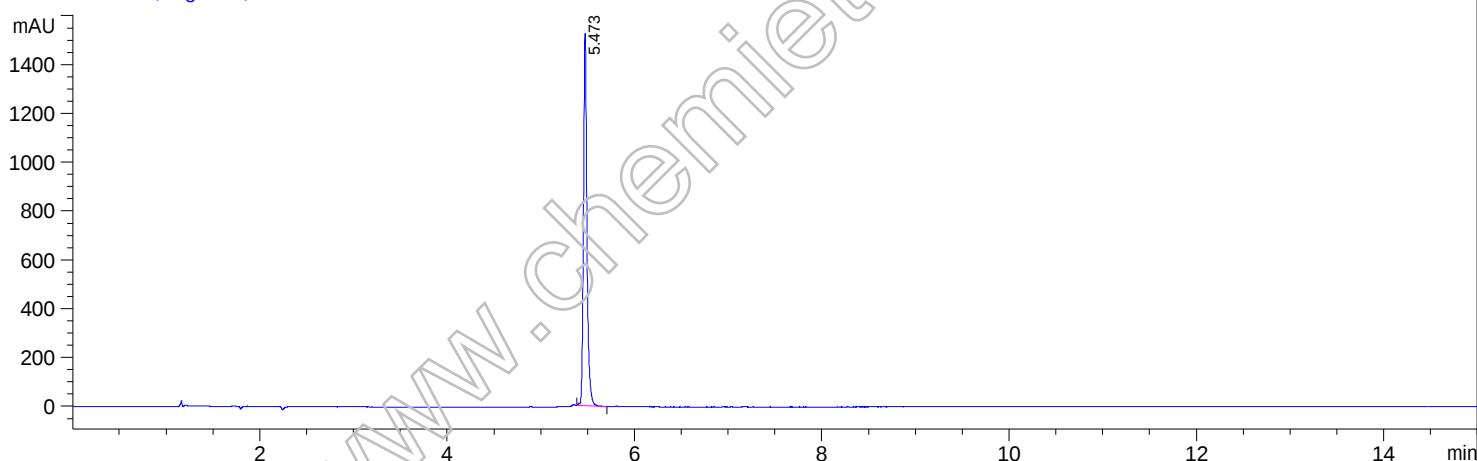


Integration Results for DAD1 A, Sig=214,4 Ref=off

| RetTim | Width | Area    | Height  | Area%  |
|--------|-------|---------|---------|--------|
| 5.47   | 0.04  | 4050.83 | 1599.35 | 100.00 |

Integration Results for DAD1 B, Sig=254,4 Ref=off

| RetTim | Width | Area    | Height  | Area%  |
|--------|-------|---------|---------|--------|
| 5.47   | 0.04  | 3923.98 | 1526.40 | 100.00 |

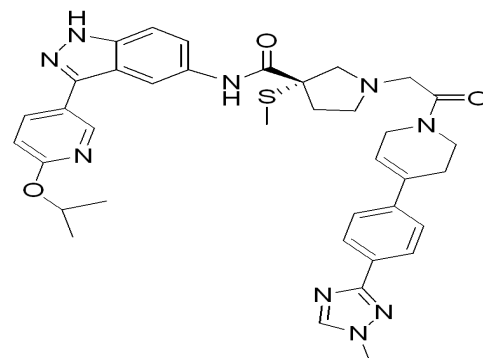

Ret. Time: 5.48

&lt;&lt;&lt;&lt; POSITIVE SPECTRA &gt;&gt;&gt;&gt;

