



Sample Name : CT-SCH353 01

Location : v1-C-12

Acq. Operator : A2-AdMIN

Inj : 0

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : D:\METHODS\QC-HPLC-15MIN.M

Analysis Method : D:\METHODS\QC-HPLC-15MIN.M

Sample Info : QC 15min Method: 'QC-HPLC-15MIN.M' 691.00

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)


Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.

Flow Rate: 1.0ml/min


Column: [REDACTED]

Column Temperature: 45 C

DAD1 A, Sig=214,4 Ref=off

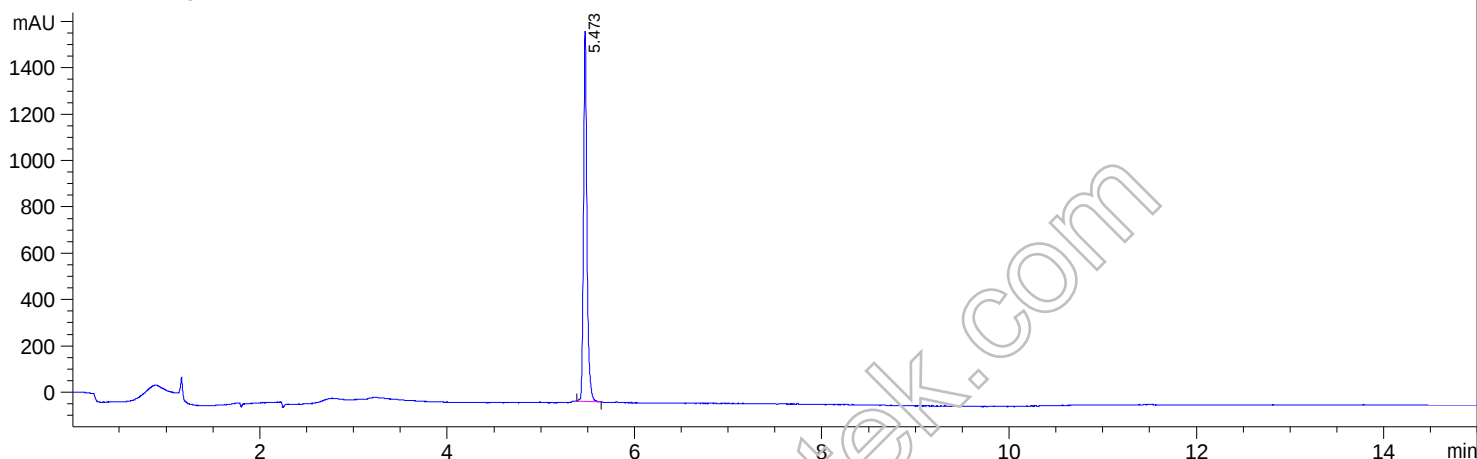

DAD1 B, Sig=254,4 Ref=off

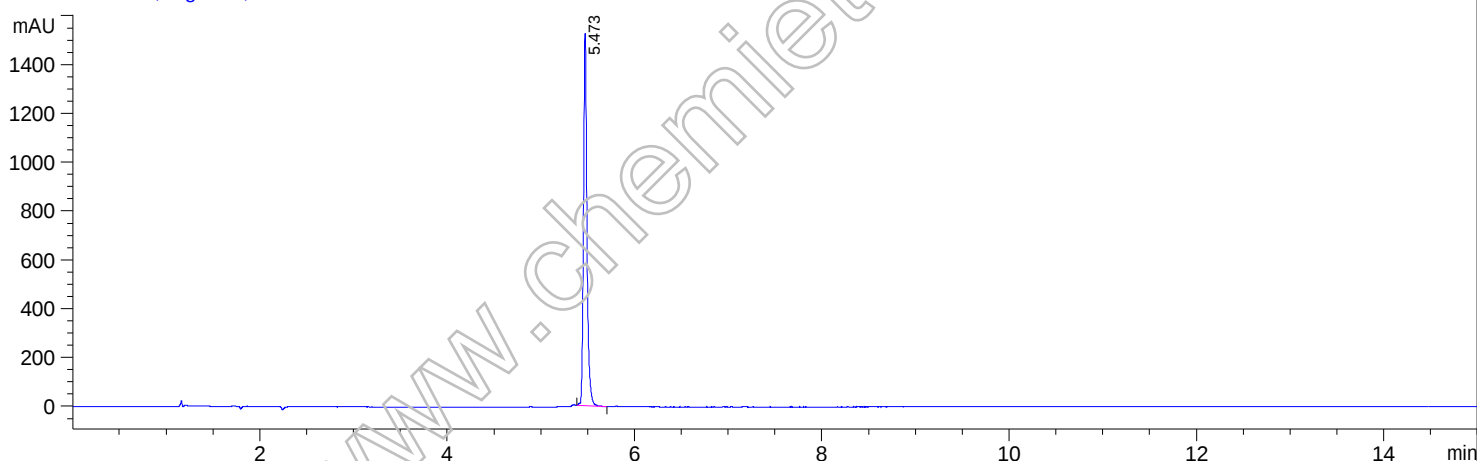


Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.47	0.04	4050.83	1599.35	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.47	0.04	3923.98	1526.40	100.00

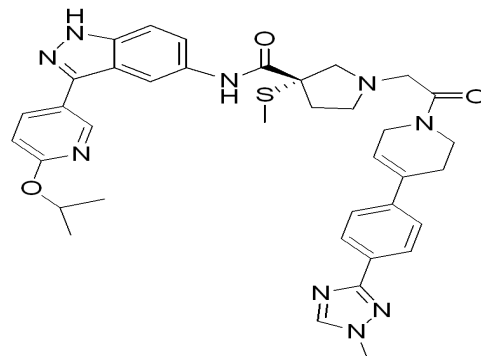

Ret. Time: 5.48

<<<< POSITIVE SPECTRA >>>>

