



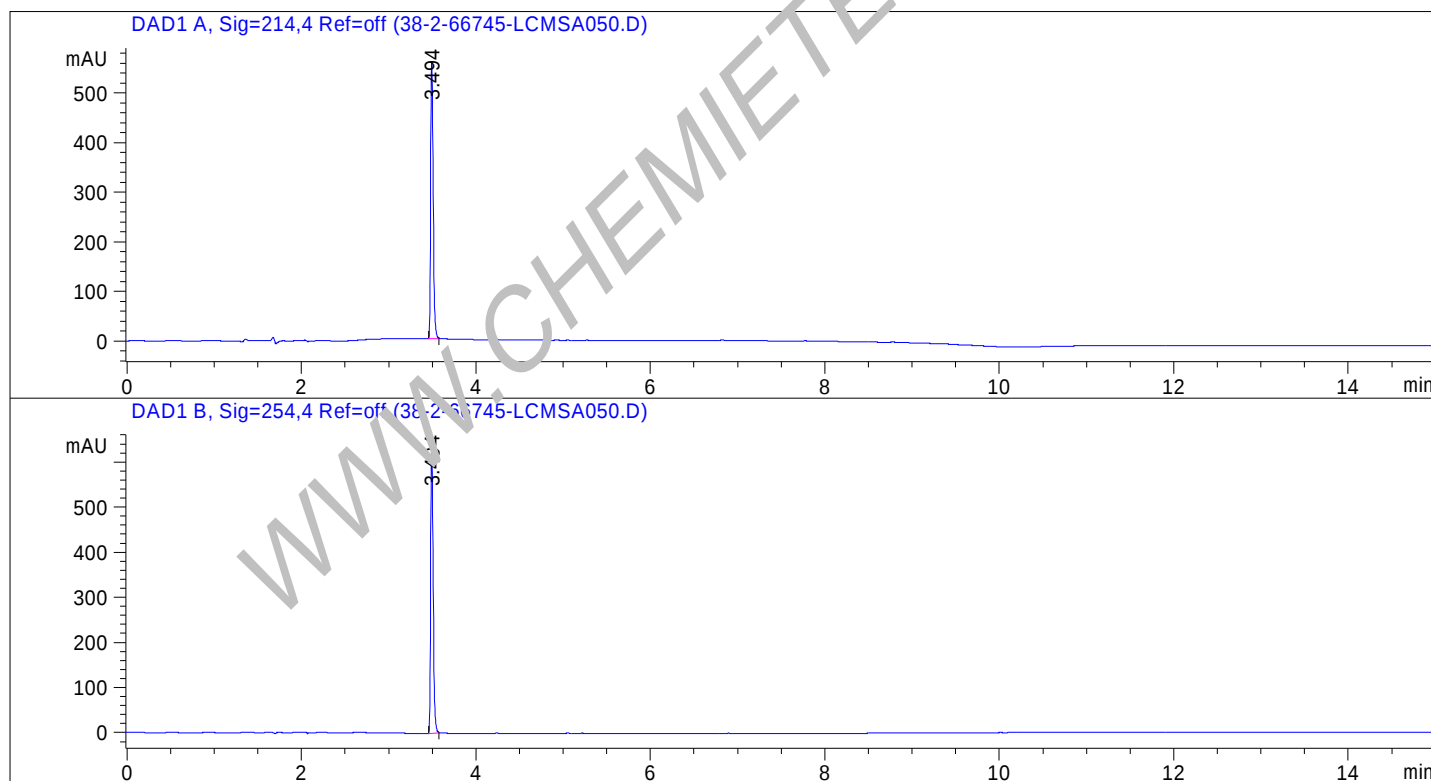

Acq. Operator: Admin
Acq. Instrument: LCMSA050
Location: P2-D-04

Acq. Method: D:\METHODS\CHEMIELAB-HPLC-15MIN.M

Analysis Method: D:\METHODS\CHEMIELAB-HPLC-15MIN.M
Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Method Info: Default
Flow Rate: 1.0ml/min
Column: Zorbax Eclipse Plus C18, 4.6*150mm, 3.5um

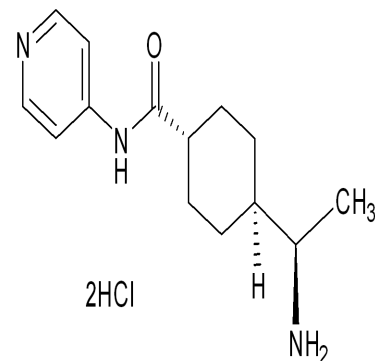

Sample Name: Y-27632, Lot 01

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.494	BB	0.0304	1119.59766	558.39172	100.0000

Totals : 1119.59766 558.39172

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.494	BB	0.0304	1264.39404	631.54163	100.0000

Totals : 1264.39404 631.54163

=====
*** End of Report ***
=====